

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027452.D
 Acq On : 07 Sep 2023 21:46
 Operator : MA/JU
 Sample : 04123-13
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9Y1

Quant Time: Sep 08 01:57:58 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	8619	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	29782	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	17360	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	36923	0.400	ng/ul	0.00
17) Chrysene-d12	21.603	240	24920	0.400	ng/ul	0.00
23) Perylene-d12	24.117	264	24715	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	48921	4.267	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	14801	0.327	ng/ul	0.00
18) Fluoranthene-d10	19.446	212	36193	0.424	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.817	202	4620	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.957	252	7789	0.085	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027452.D
Acq On : 07 Sep 2023 21:46
Operator : MA/JU
Sample : 04123-13
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9Y1

Quant Time: Sep 08 01:57:58 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




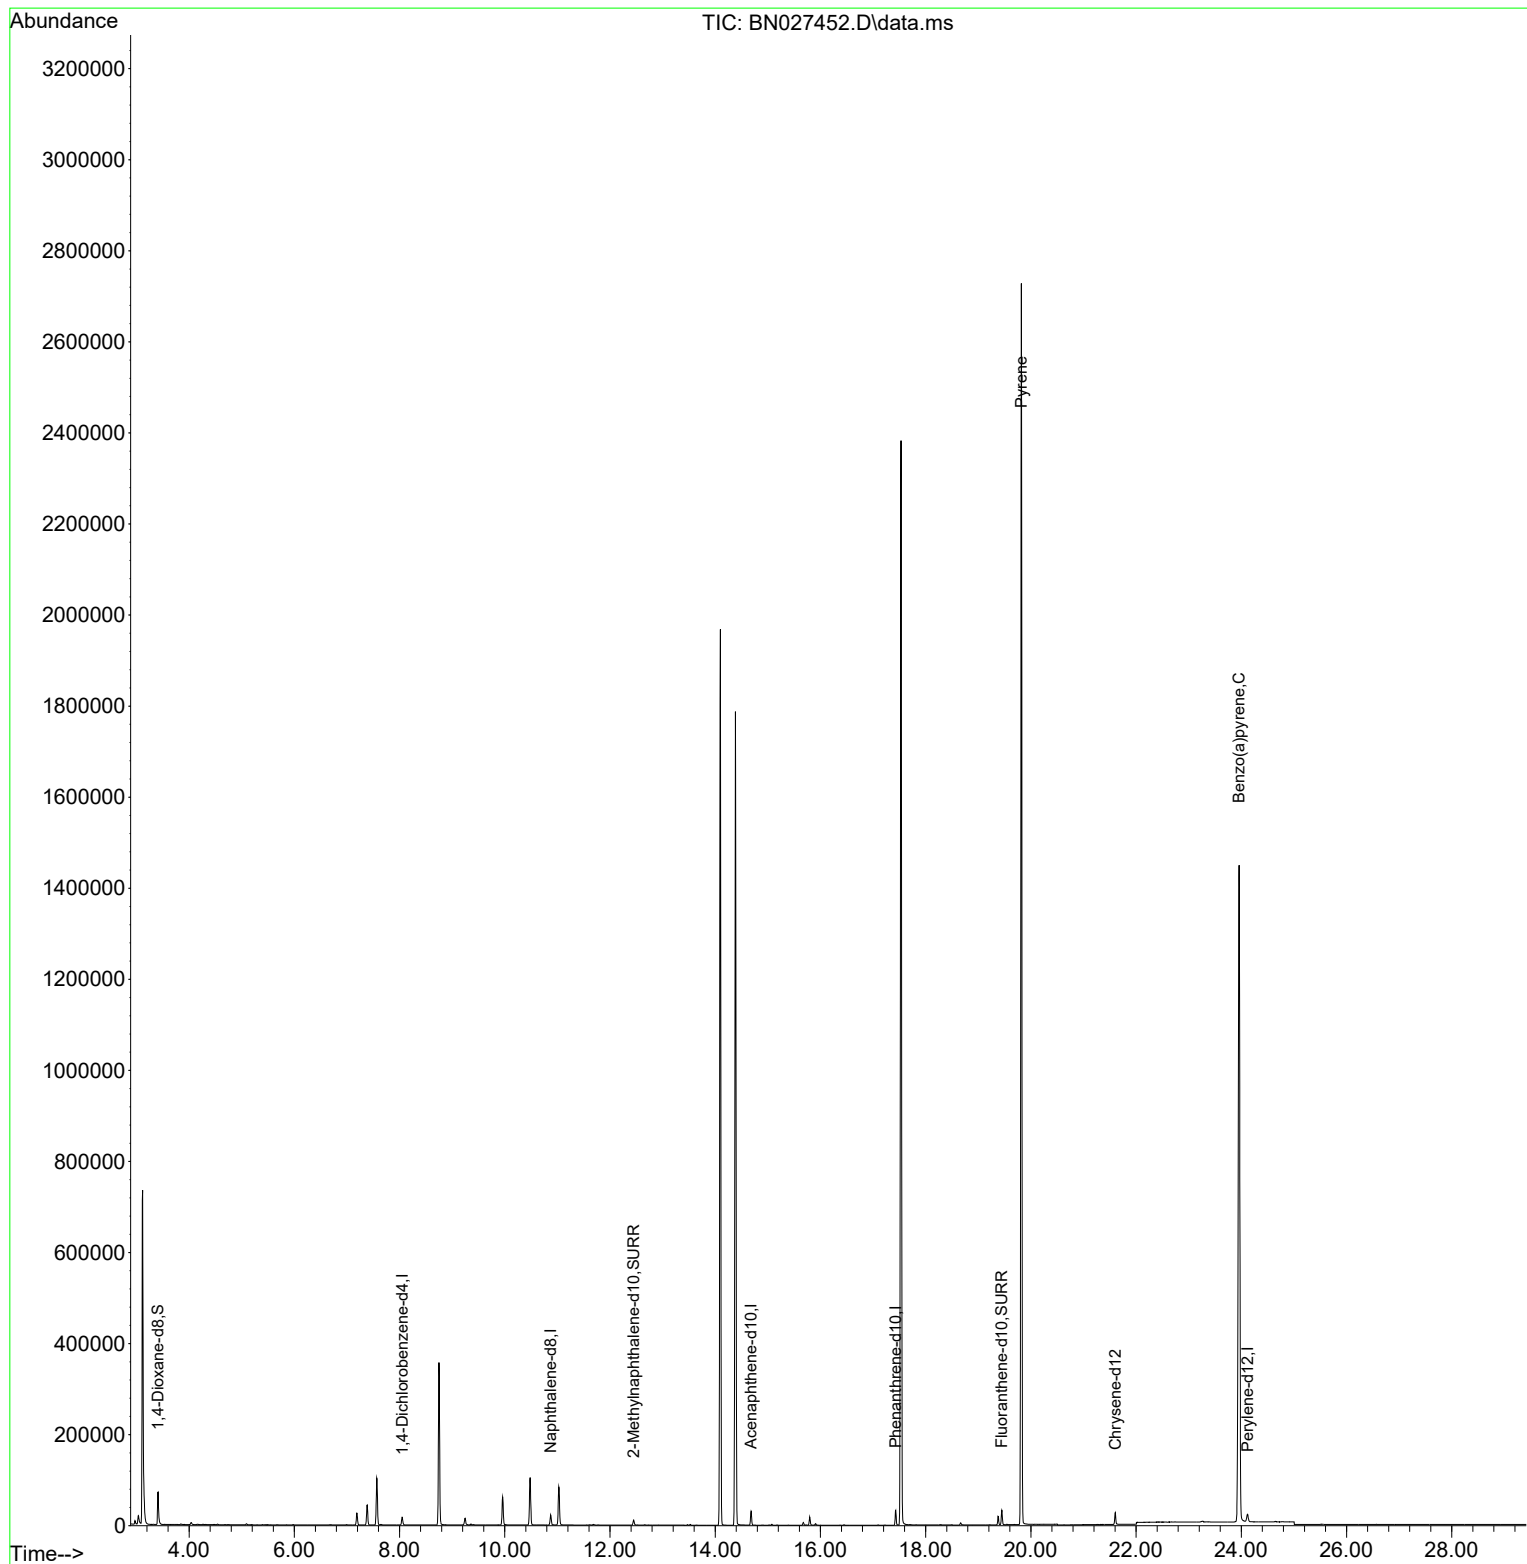


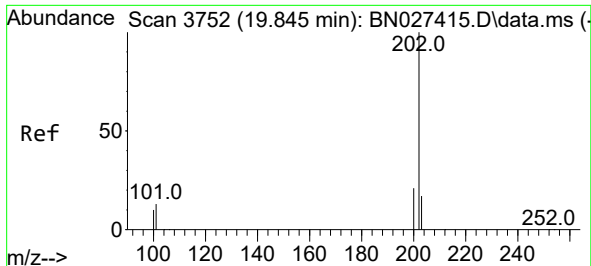

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.817 min Scan# 31
Delta R.T. -0.032 min
Lab File: BN027452.D
Acq: 07 Sep 2023 21:46

Instrument :
BNA_N
ClientSampleId :
BH9Y1

Tgt Ion:202 Resp: 4620
Ion Ratio Lower Upper
202 100
101 149.8 11.4 17.2#
100 1107.1 9.4 14.2#

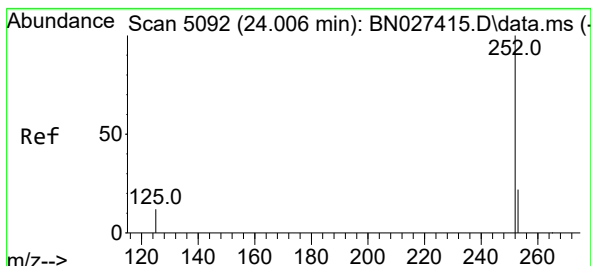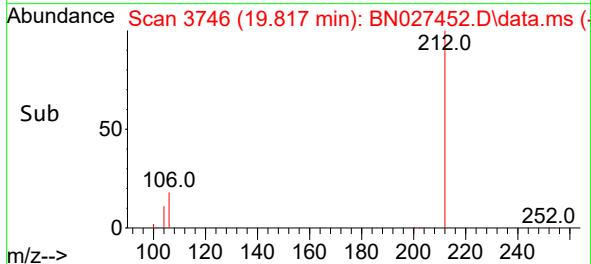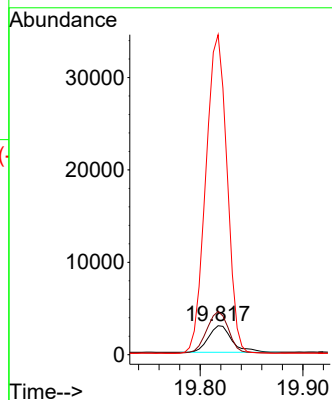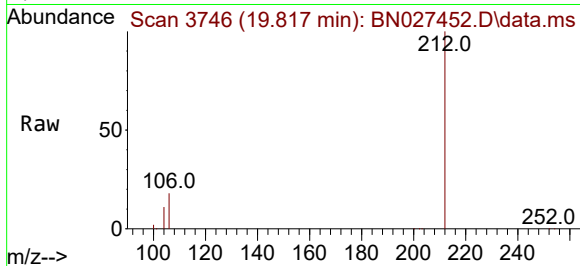

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.957 min Scan# 5075
Delta R.T. -0.061 min
Lab File: BN027452.D
Acq: 07 Sep 2023 21:46

Tgt Ion:252 Resp: 7789
Ion Ratio Lower Upper
252 100
253 52.0 22.4 33.6#
125 49.0 17.4 26.2#

