




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027449.D
Acq On : 07 Sep 2023 19:53
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH930

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:57:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :mohammad ahmed 09/09/2023

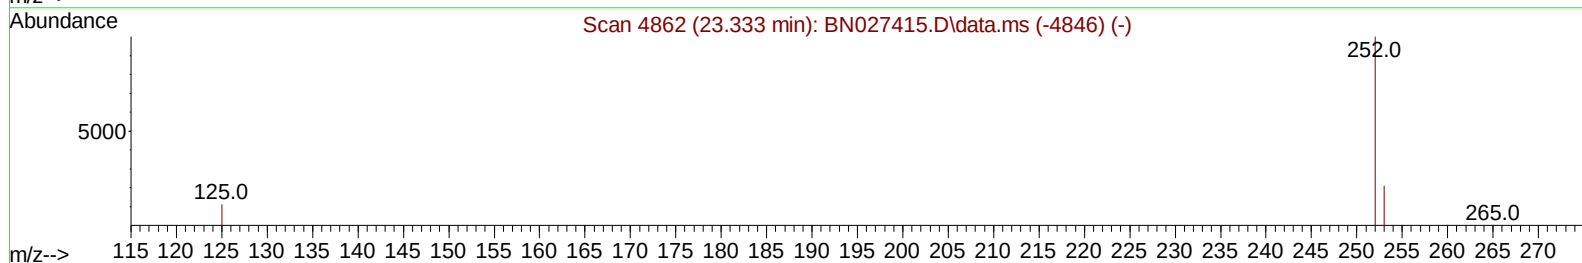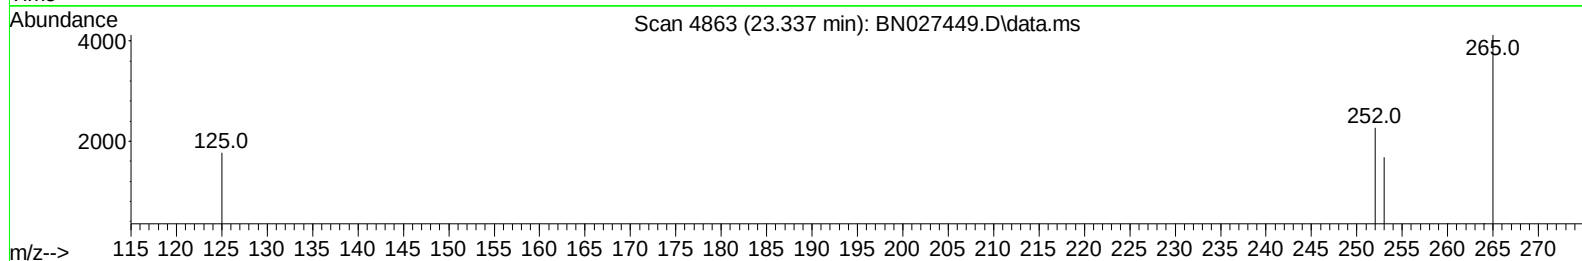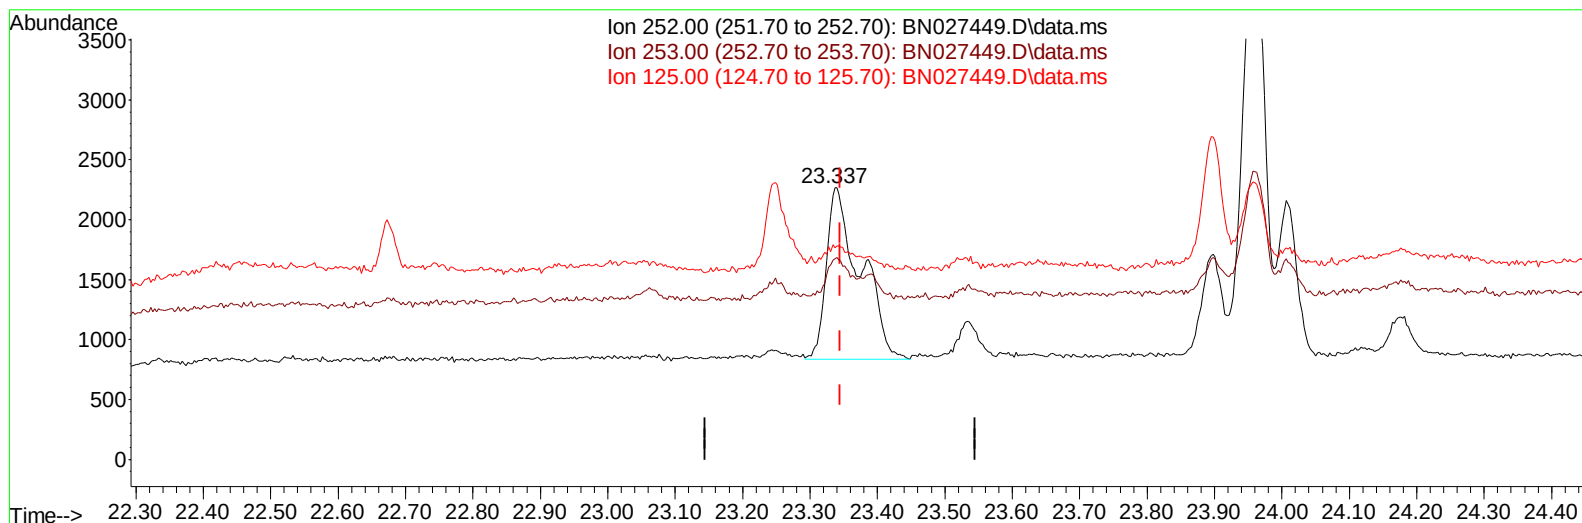

TIC: BN027449.D\data.ms

(24) Benzo(b)fluoranthene

23.337min (-0.009) 0.04 ng/u1

response 5014

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.80	73.96#
125.00	16.90	77.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027449.D
Acq On : 07 Sep 2023 19:53
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH930

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:57:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :mohammad ahmed 09/09/2023

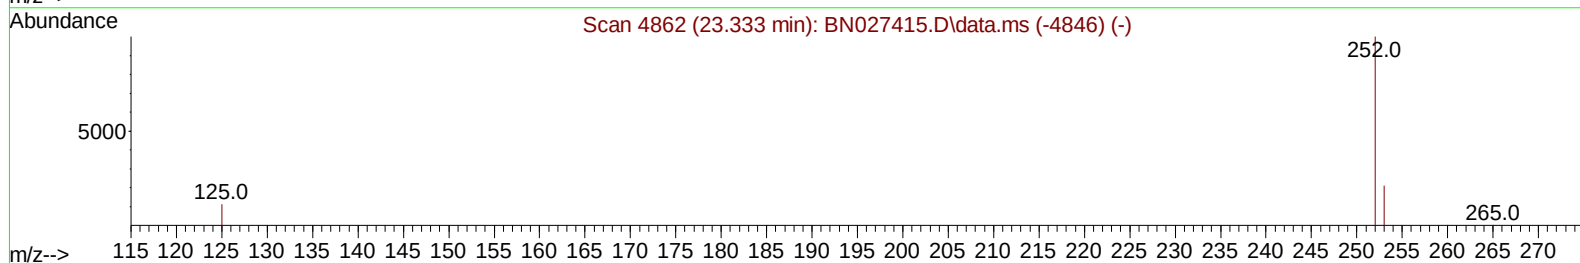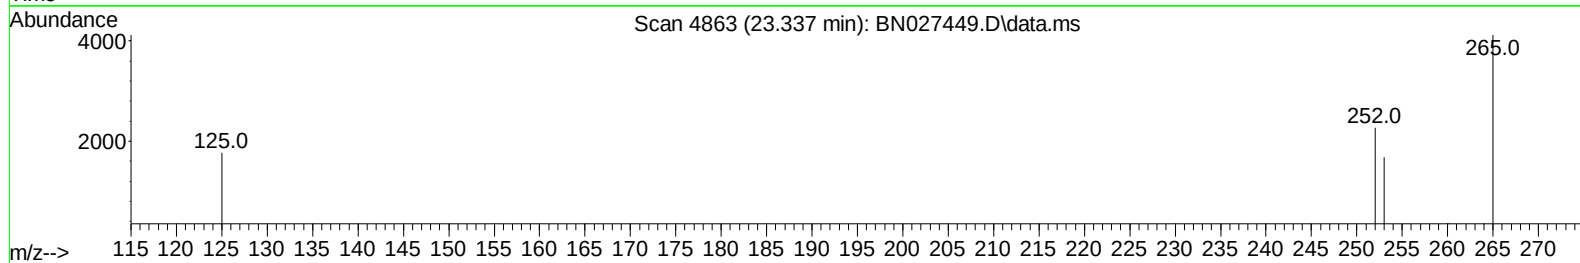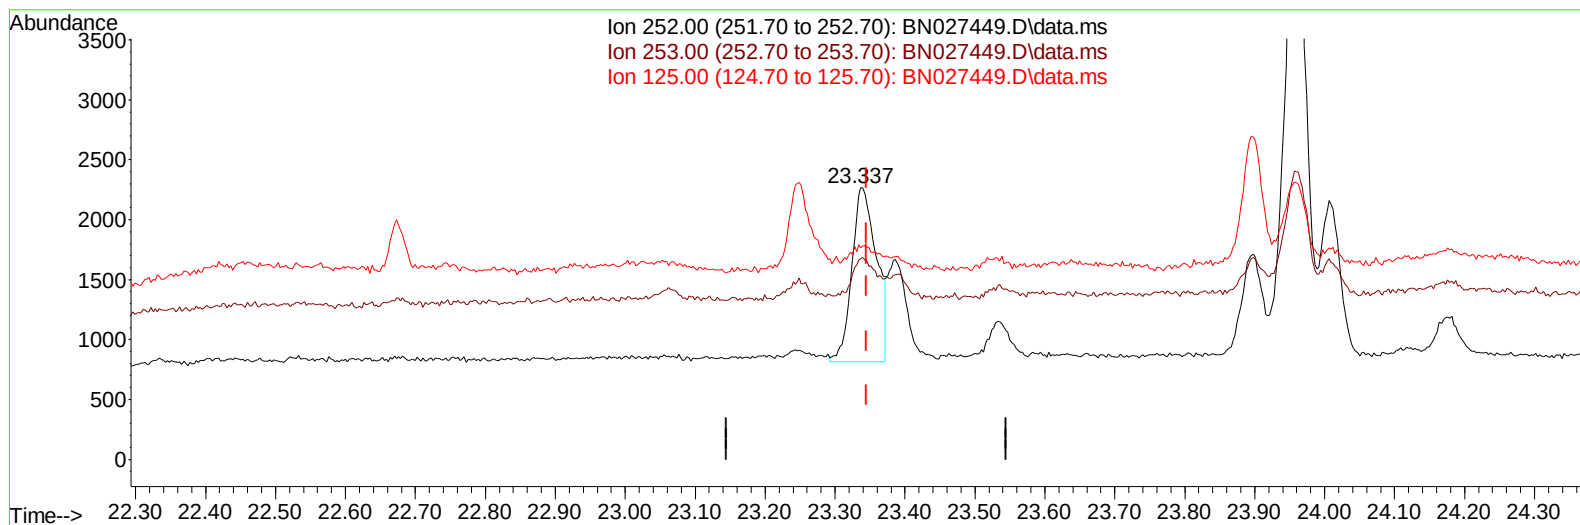

TIC: BN027449.D\data.ms

(24) Benzo(b)fluoranthene

23.337min (-0.009) 0.03 ng/ul m

response 3579

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	24.80	73.96#
125.00	16.90	77.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027449.D
 Acq On : 07 Sep 2023 19:53
 Operator : MA/JU
 Sample : 04123-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH930

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/08/2023
 Supervised By :mohammad ahmed 09/09/2023

Quant Time: Sep 08 01:57:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.051	152		10083	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136		34769	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.684	164		20314	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188		42981	0.400	ng/ul	0.00
17) Chrysene-d12	21.606	240		27200	0.400	ng/ul	0.00
23) Perylene-d12	24.117	264		26493	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.410	96		59472	4.434	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152		17409	0.330	ng/ul	0.00
18) Fluoranthene-d10	19.450	212		40224	0.432	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.448	88		511	0.038	ng/ul#	41
15) Phenanthrene	17.472	178		3035	0.022	ng/ul#	87
19) Fluoranthene	19.483	202		6184	0.049	ng/ul	97
20) Pyrene	19.850	202		5599	0.044	ng/ul	96
21) Benzo(a)anthracene	21.589	228		3048	0.031	ng/ul#	66
24) Benzo(b)fluoranthene	23.337	252		3579m	0.029	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027449.D
Acq On : 07 Sep 2023 19:53
Operator : MA/JU
Sample : 04123-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH930

Manual IntegrationsAPPROVED

Quant Time: Sep 08 01:57:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/08/2023
Supervised By :mohammad ahmed 09/09/2023

