

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027413.D
 Acq On : 06 Sep 2023 18:53
 Operator : MA/JU
 Sample : 04148-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH8S3

Quant Time: Sep 06 23:25:14 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	7513	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	26318	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	16591	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	38082	0.400	ng/ul	0.00
17) Chrysene-d12	21.606	240	30429	0.400	ng/ul	0.00
23) Perylene-d12	24.117	264	31684	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	48491	4.852	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	12605	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	36000	0.345	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	5366	0.531	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027413.D
Acq On : 06 Sep 2023 18:53
Operator : MA/JU
Sample : 04148-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH8S3

Quant Time: Sep 06 23:25:14 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

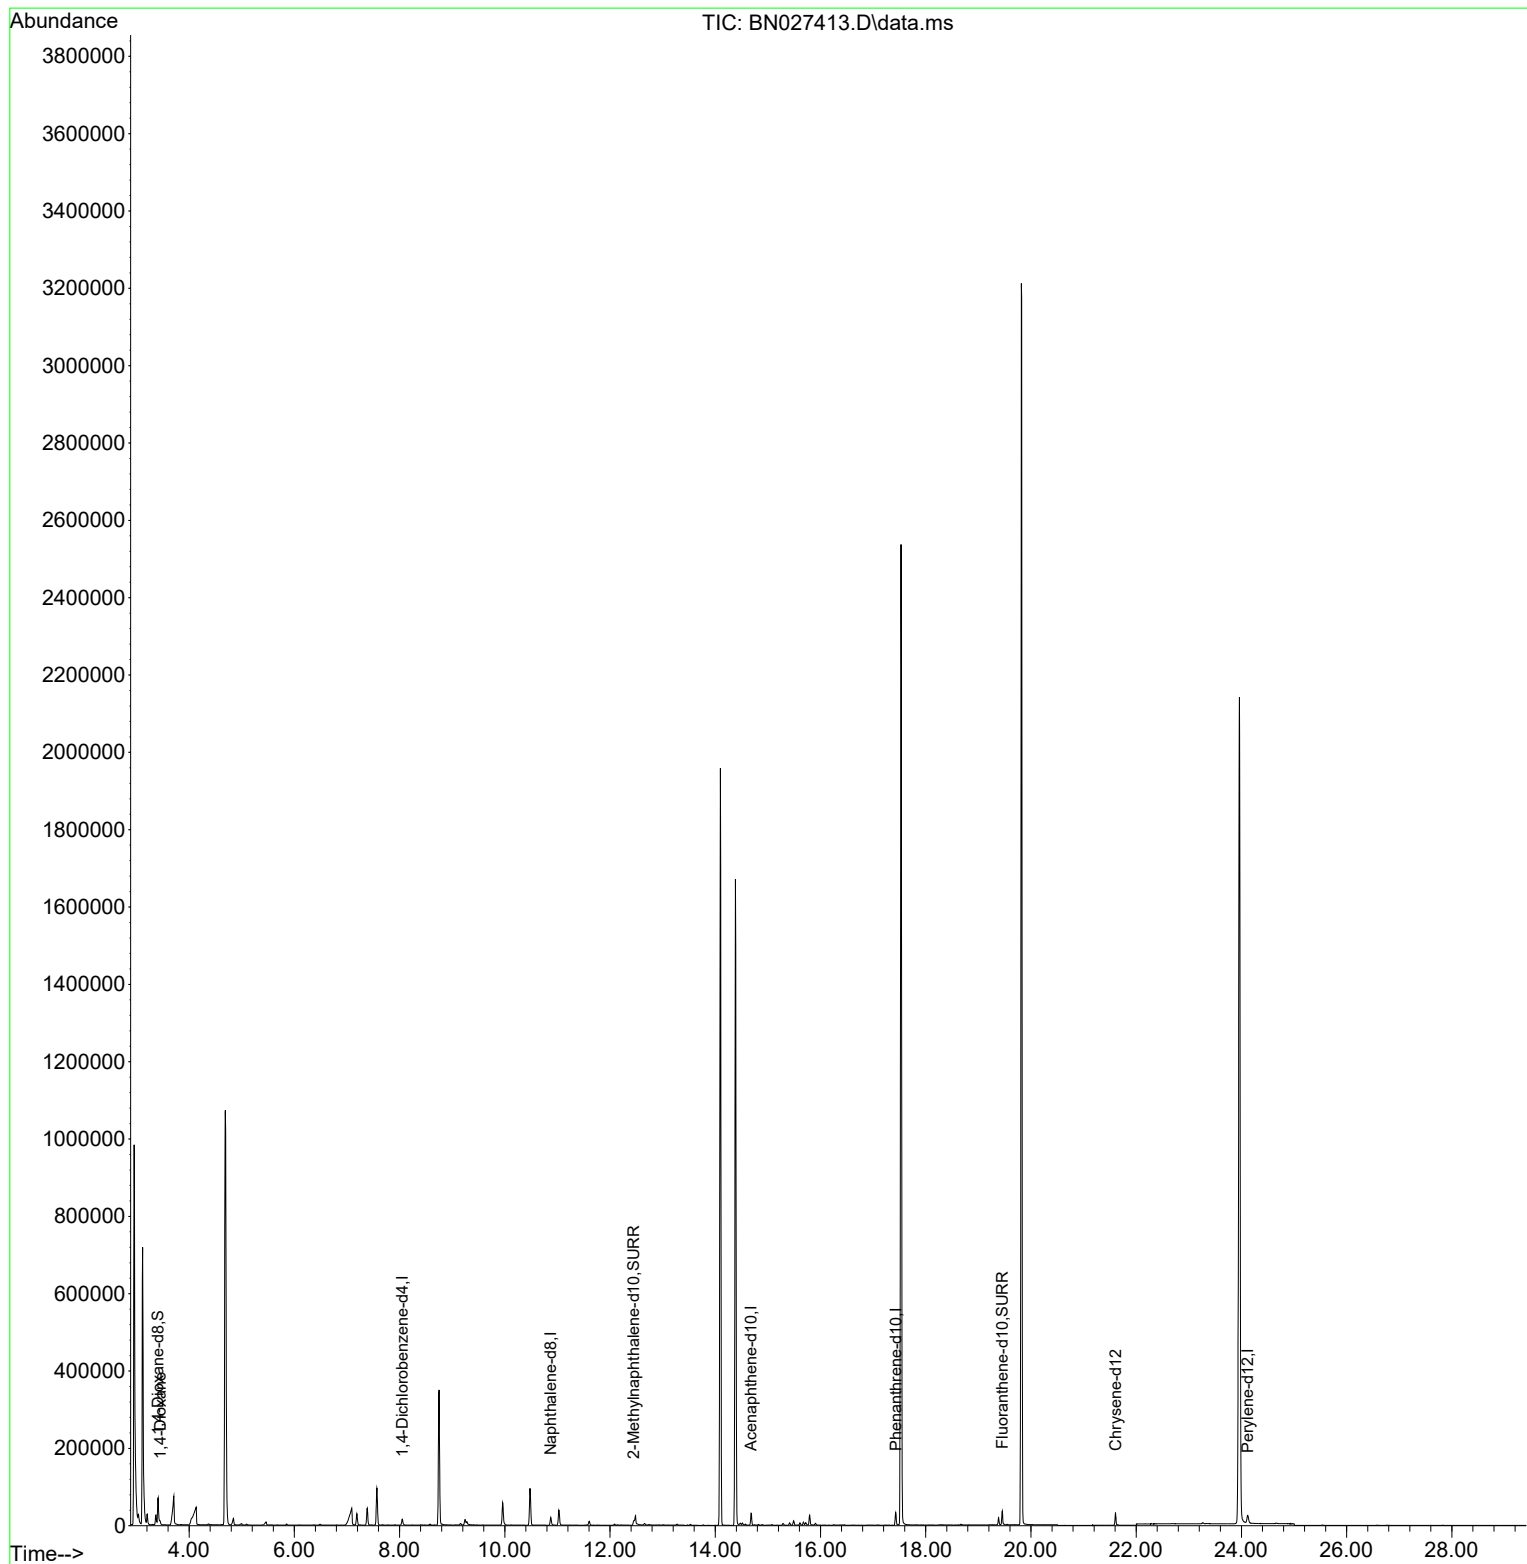

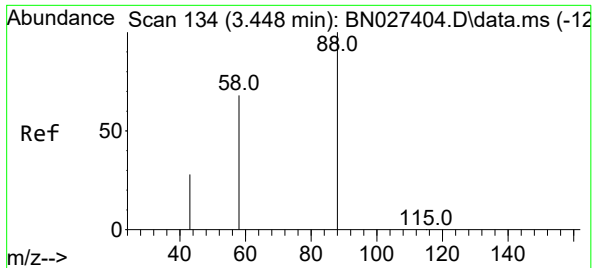

1,4-Dioxane
 Concen: 0.531 ng/ul
 RT: 3.448 min Scan# 11
 Delta R.T. -0.008 min
 Lab File: BN027413.D
 Acq: 06 Sep 2023 18:53

Instrument :
 BNA_N
 ClientSampleId :
 BH8S3

Tgt Ion:	88	Resp:	5366
Ion	Ratio	Lower	Upper
88	100		
43	37.6	26.8	40.2
58	61.7	39.9	59.9

