

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027418.D
 Acq On : 06 Sep 2023 22:40
 Operator : MA/JU
 Sample : 04148-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJW3

Quant Time: Sep 06 23:26:14 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	5938	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	21359	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	13762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	30187	0.400	ng/ul	-0.01
17) Chrysene-d12	21.600	240	25036	0.400	ng/ul	0.00
23) Perylene-d12	24.111	264	26495	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	39045	4.943	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	12129	0.374	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	33254	0.388	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	2999	0.375	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027418.D
Acq On : 06 Sep 2023 22:40
Operator : MA/JU
Sample : 04148-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJW3

Quant Time: Sep 06 23:26:14 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

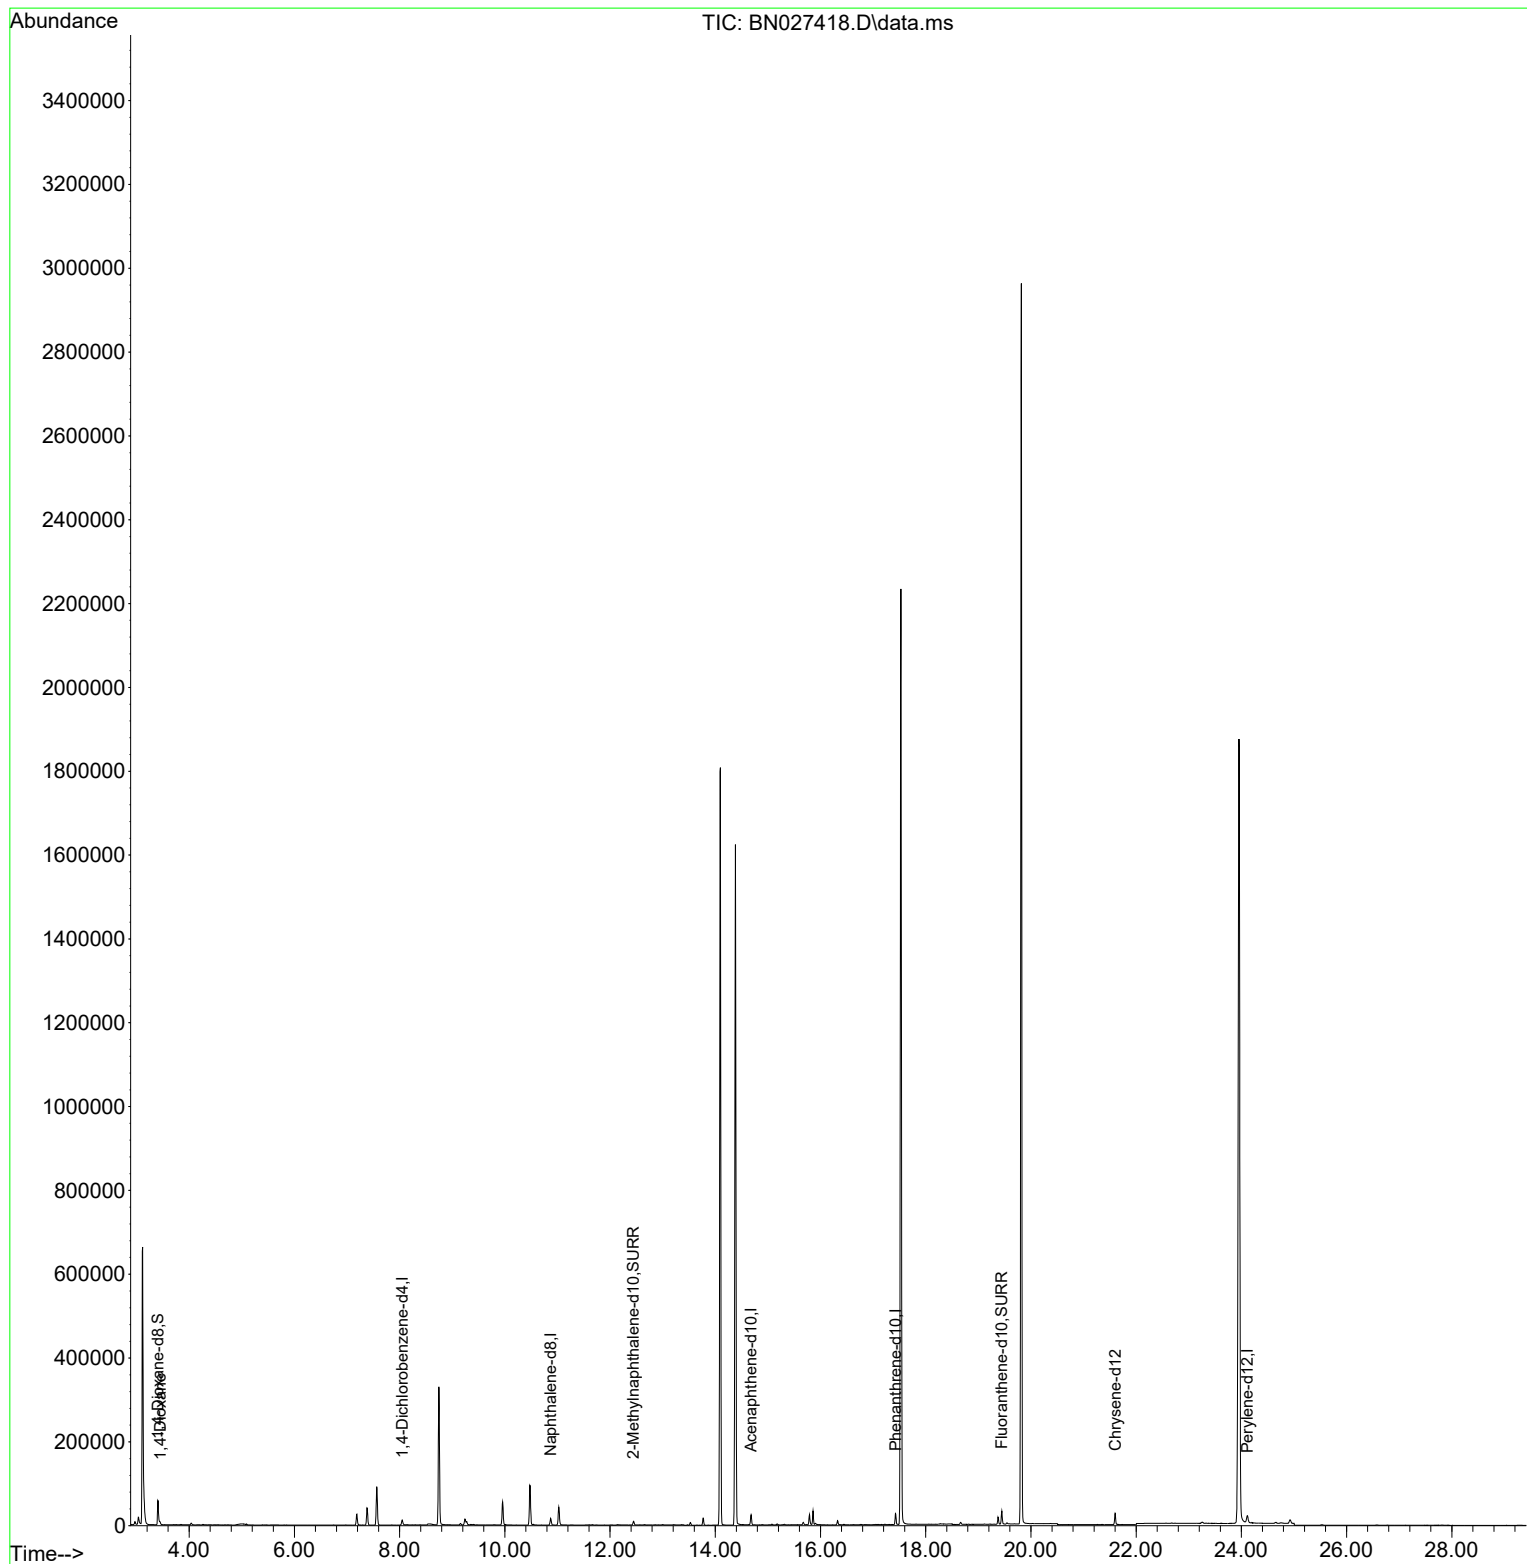

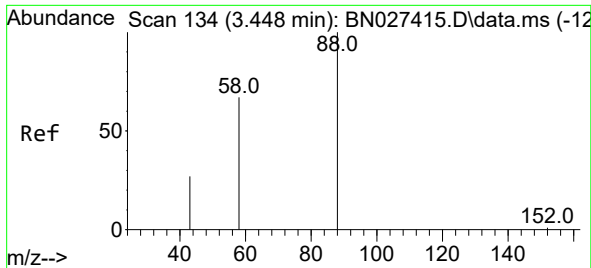

1,4-Dioxane

Concen: 0.375 ng/ul

RT: 3.448 min Scan# 11

Delta R.T. -0.009 min

Lab File: BN027418.D


Acq: 06 Sep 2023 22:40

Instrument :

BNA_N

ClientSampleId :

BBJW3

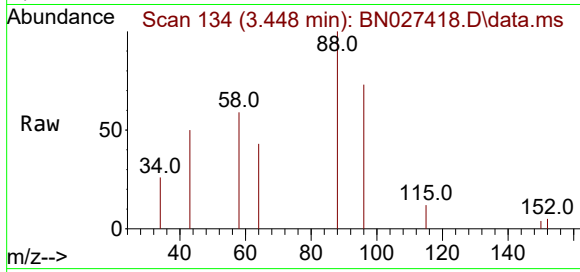

Tgt Ion: 88 Resp: 2999

Ion Ratio Lower Upper

88 100

43 49.9 26.8 40.2#

58 59.3 39.9 59.9

