

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027420.D
 Acq On : 06 Sep 2023 23:55
 Operator : MA/JU
 Sample : 04148-12
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJW5

Quant Time: Sep 07 01:07:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	5831	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	20810	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	13167	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	28705	0.400	ng/ul	-0.01
17) Chrysene-d12	21.600	240	22960	0.400	ng/ul	0.00
23) Perylene-d12	24.111	264	24277	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	34575	4.458	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	13838	0.438	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	36461	0.463	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.443	88	13188	1.680	ng/ul#	86
14) Pentachlorophenol	17.054	266	246	0.044	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027420.D
Acq On : 06 Sep 2023 23:55
Operator : MA/JU
Sample : 04148-12
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJW5

Quant Time: Sep 07 01:07:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration




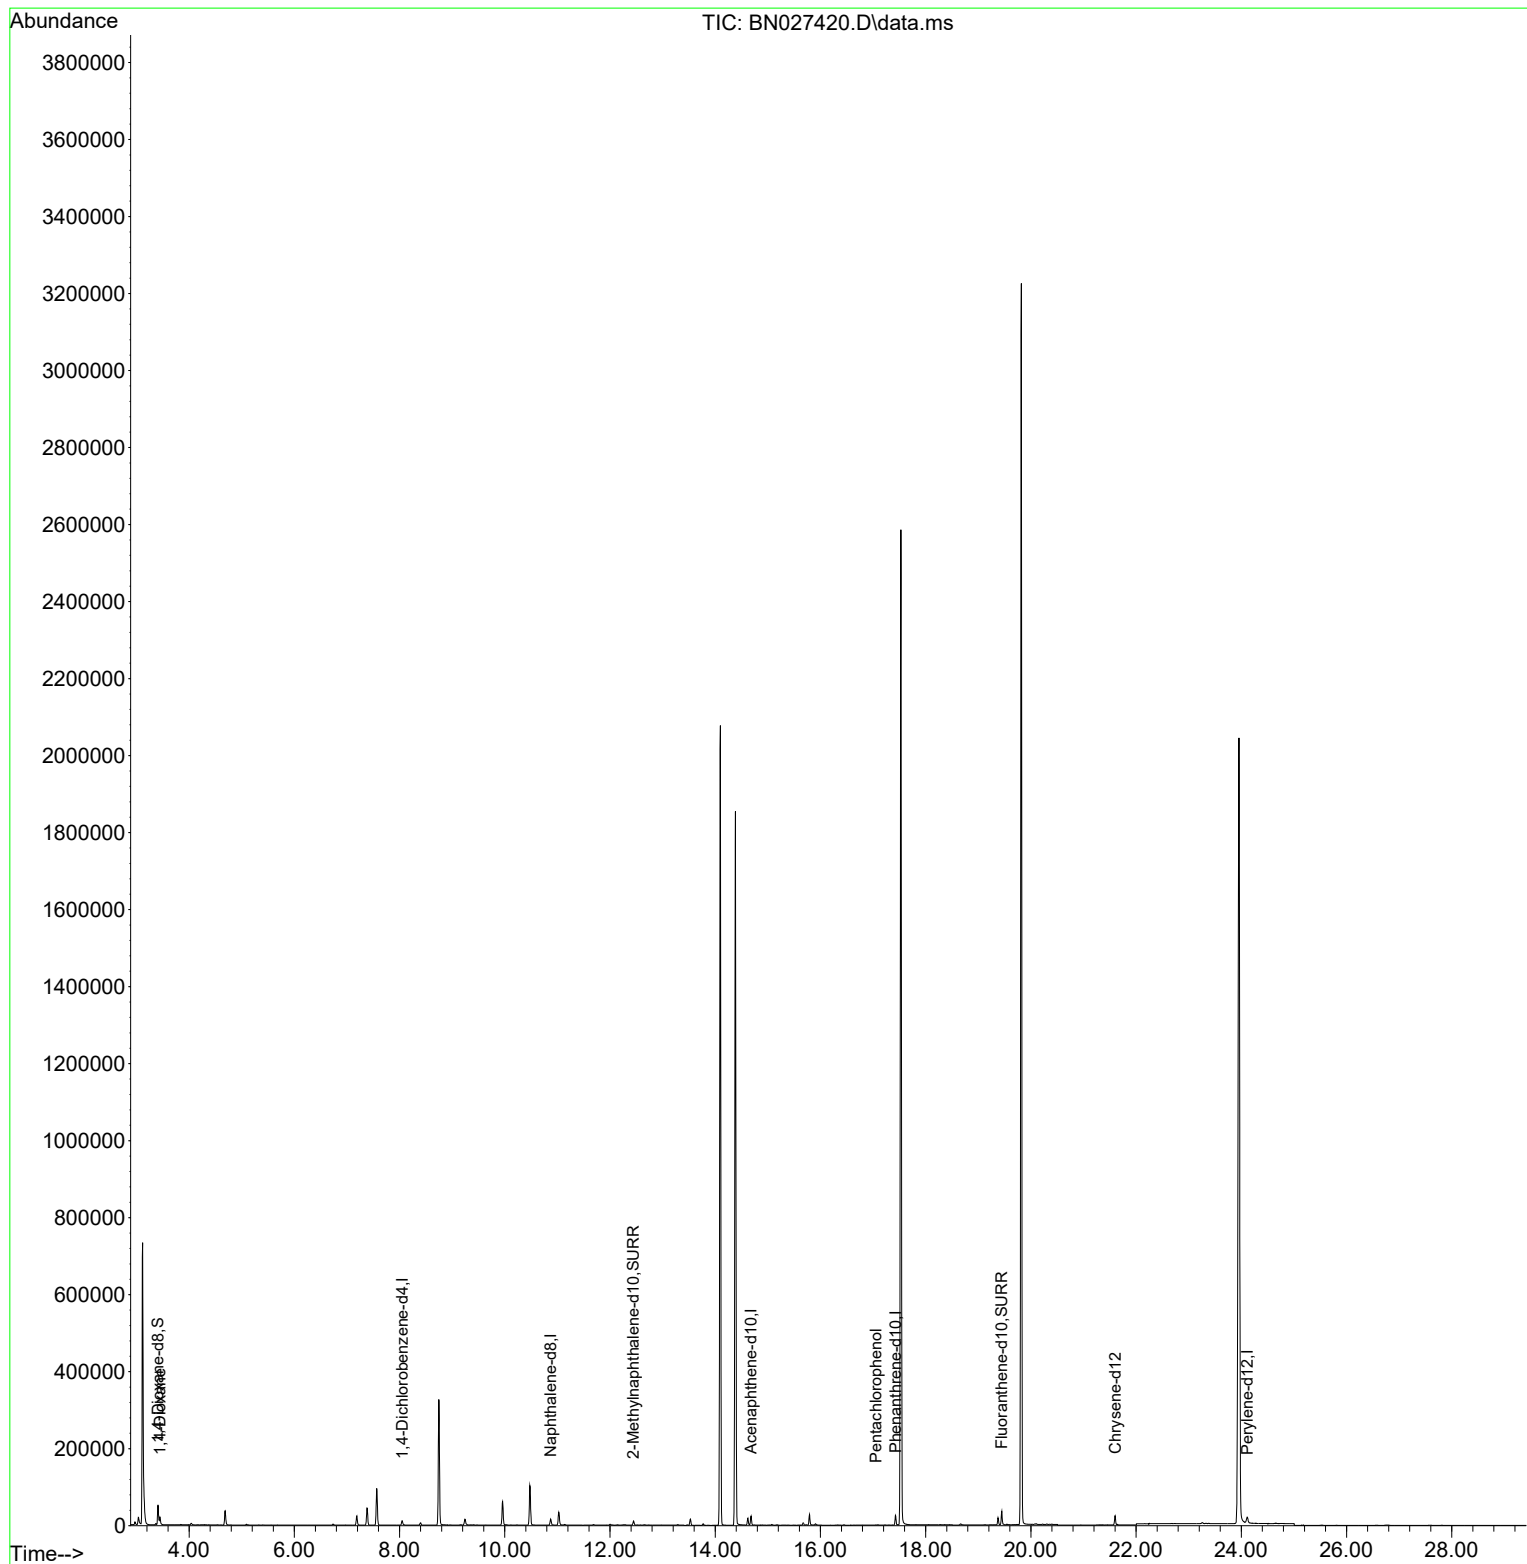


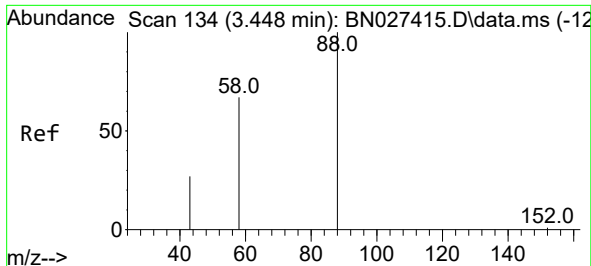

#2
1,4-Dioxane
Concen: 1.680 ng/ul
RT: 3.443 min Scan# 11
Delta R.T. -0.013 min
Lab File: BN027420.D
Acq: 06 Sep 2023 23:55

Instrument :
BNA_N
ClientSampleId :
BBJW5

Tgt Ion: 88 Resp: 13188
Ion Ratio Lower Upper
88 100
43 33.6 26.8 40.2
58 65.4 39.9 59.9#

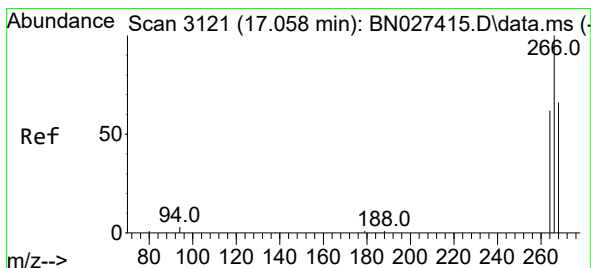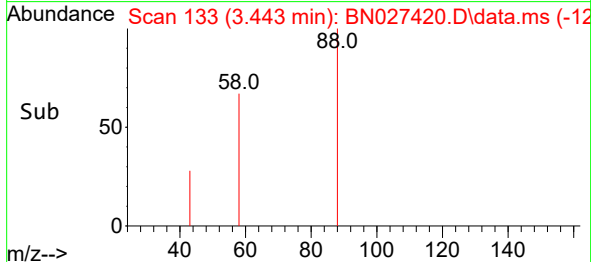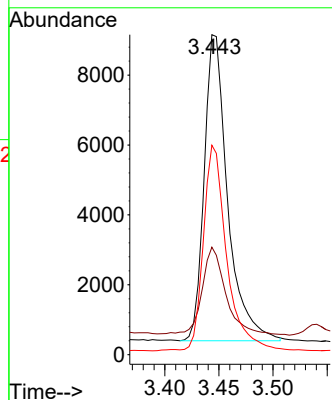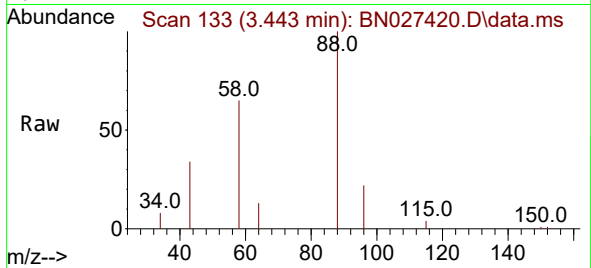

#14
Pentachlorophenol
Concen: 0.044 ng/ul
RT: 17.054 min Scan# 3120
Delta R.T. -0.012 min
Lab File: BN027420.D
Acq: 06 Sep 2023 23:55

Tgt Ion: 266 Resp: 246
Ion Ratio Lower Upper
266 100
264 58.1 50.4 75.6
268 61.0 51.9 77.9

