

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027421.D
 Acq On : 07 Sep 2023 00:33
 Operator : MA/JU
 Sample : 04123-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH920

Quant Time: Sep 07 04:37:29 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	8834	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	31396	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	19309	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	43384	0.400	ng/ul	-0.01
17) Chrysene-d12	21.597	240	34864	0.400	ng/ul	-0.01
23) Perylene-d12	24.111	264	37745	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	58304	4.962	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.445	152	16463	0.346	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	45778	0.383	ng/ul	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.448	88	1627	0.137	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027421.D
Acq On : 07 Sep 2023 00:33
Operator : MA/JU
Sample : 04123-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH920

Quant Time: Sep 07 04:37:29 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

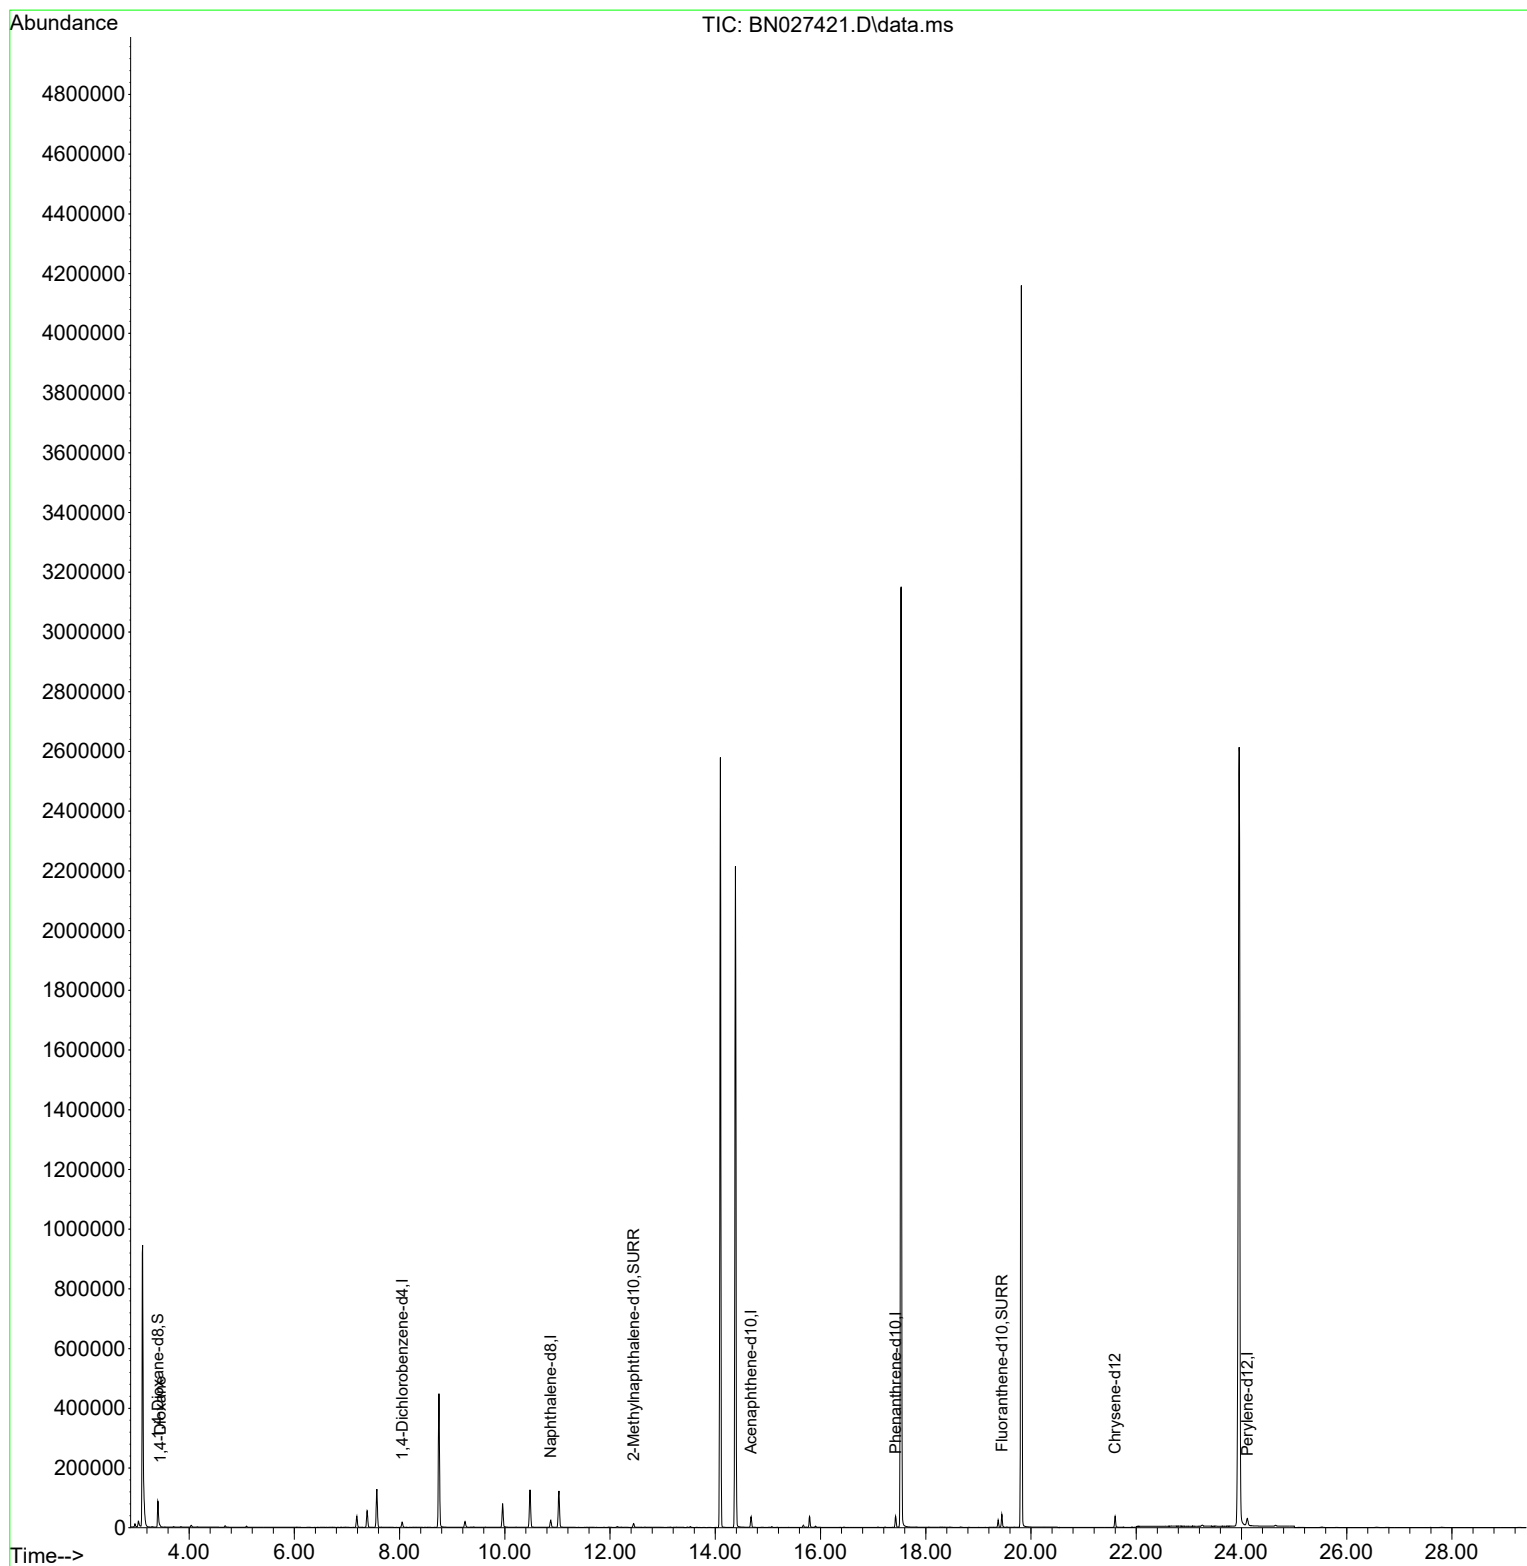

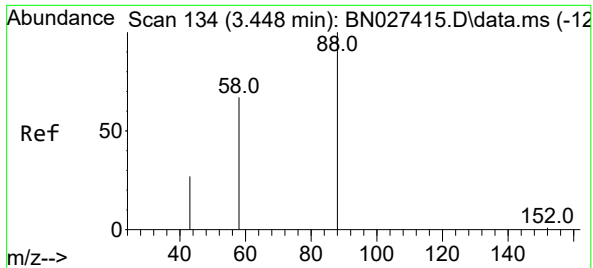

1,4-Dioxane
 Concen: 0.137 ng/ul
 RT: 3.448 min Scan# 11
 Delta R.T. -0.009 min
 Lab File: BN027421.D
 Acq: 07 Sep 2023 00:33

Instrument :
 BNA_N
 ClientSampleId :
 BH920

Tgt Ion: 88 Resp: 1627
 Ion Ratio Lower Upper
 88 100
 43 52.5 26.8 40.2#
 58 55.4 39.9 59.9

