

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027422.D
 Acq On : 07 Sep 2023 01:10
 Operator : MA/JU
 Sample : 04123-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH923

Quant Time: Sep 07 04:37:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	8397	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.872	136	30047	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	18186	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	40336	0.400	ng/ul	-0.01
17) Chrysene-d12	21.601	240	32493	0.400	ng/ul	0.00
23) Perylene-d12	24.114	264	34495	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	51736	4.632	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	15103	0.331	ng/ul	-0.01
18) Fluoranthene-d10	19.446	212	38518	0.346	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	2039	0.180	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027422.D
Acq On : 07 Sep 2023 01:10
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH923

Quant Time: Sep 07 04:37:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

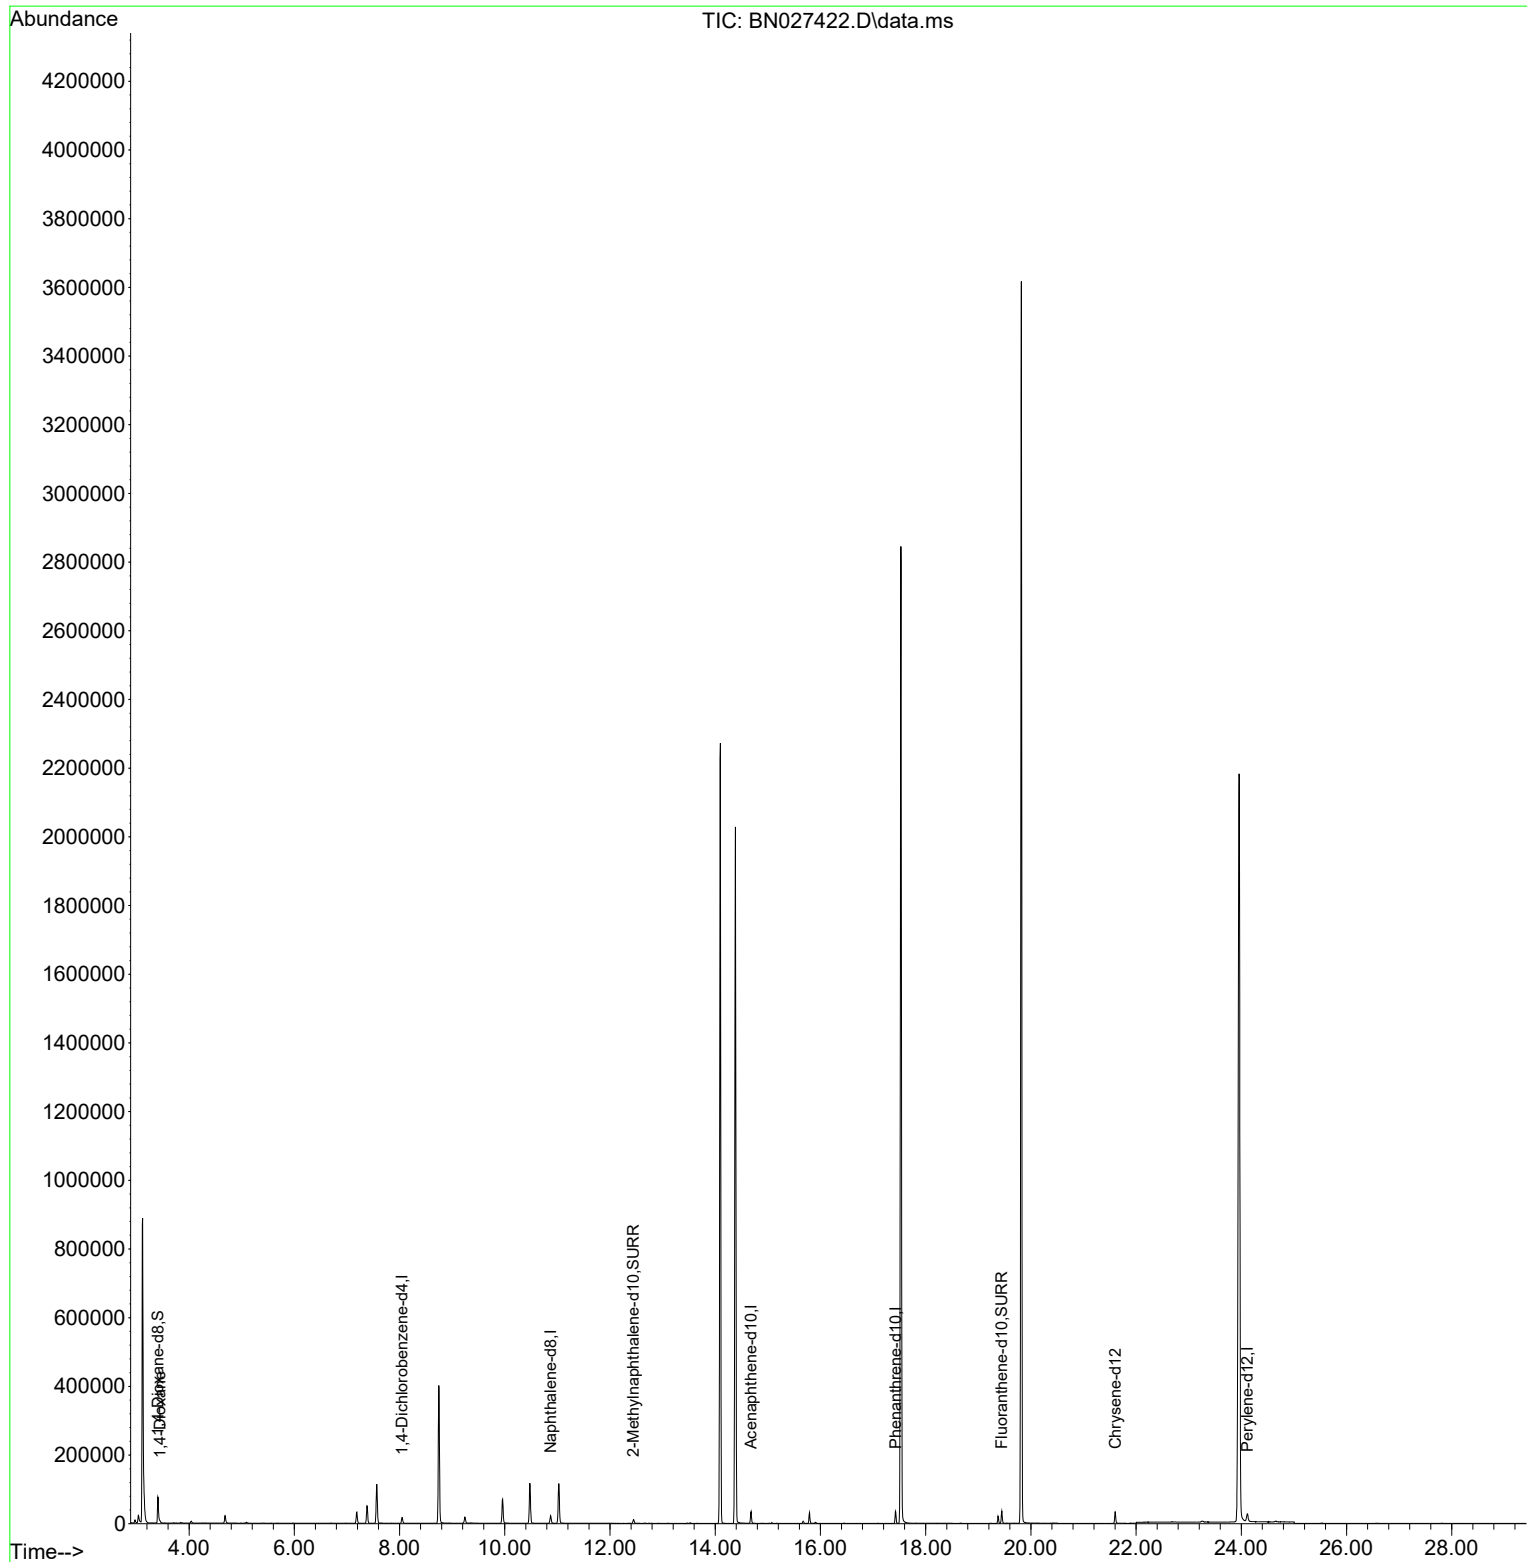

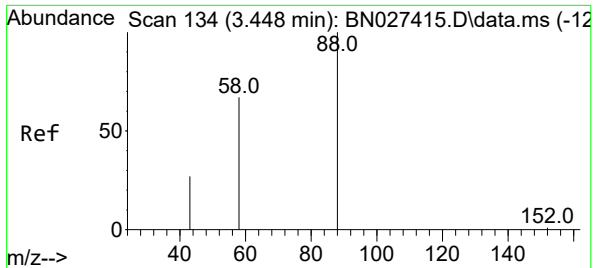

1,4-Dioxane
 Concen: 0.180 ng/ul
 RT: 3.444 min Scan# 11
 Delta R.T. -0.013 min
 Lab File: BN027422.D
 Acq: 07 Sep 2023 01:10

Instrument :
 BNA_N
 ClientSampleId :
 BH923

Tgt Ion: 88	Resp: 2039
Ion Ratio	Lower Upper
88	100
43	51.9 26.8 40.2#
58	59.1 39.9 59.9

