

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027423.D
 Acq On : 07 Sep 2023 01:47
 Operator : MA/JU
 Sample : 04123-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH942

Quant Time: Sep 07 04:42:50 2023
 Quant Title :
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	8843	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	31199	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	19106	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	42060	0.400	ng/ul	-0.01
17) Chrysene-d12	21.600	240	34921	0.400	ng/ul	0.00
23) Perylene-d12	24.111	264	37749	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	49054	4.170	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.445	152	14261	0.301	ng/ul	-0.01
18) Fluoranthene-d10	19.446	212	40752	0.341	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.443	88	24609	2.067	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027423.D
Acq On : 07 Sep 2023 01:47
Operator : MA/JU
Sample : 04123-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH942

Quant Time: Sep 07 04:42:50 2023
Quant Title :
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

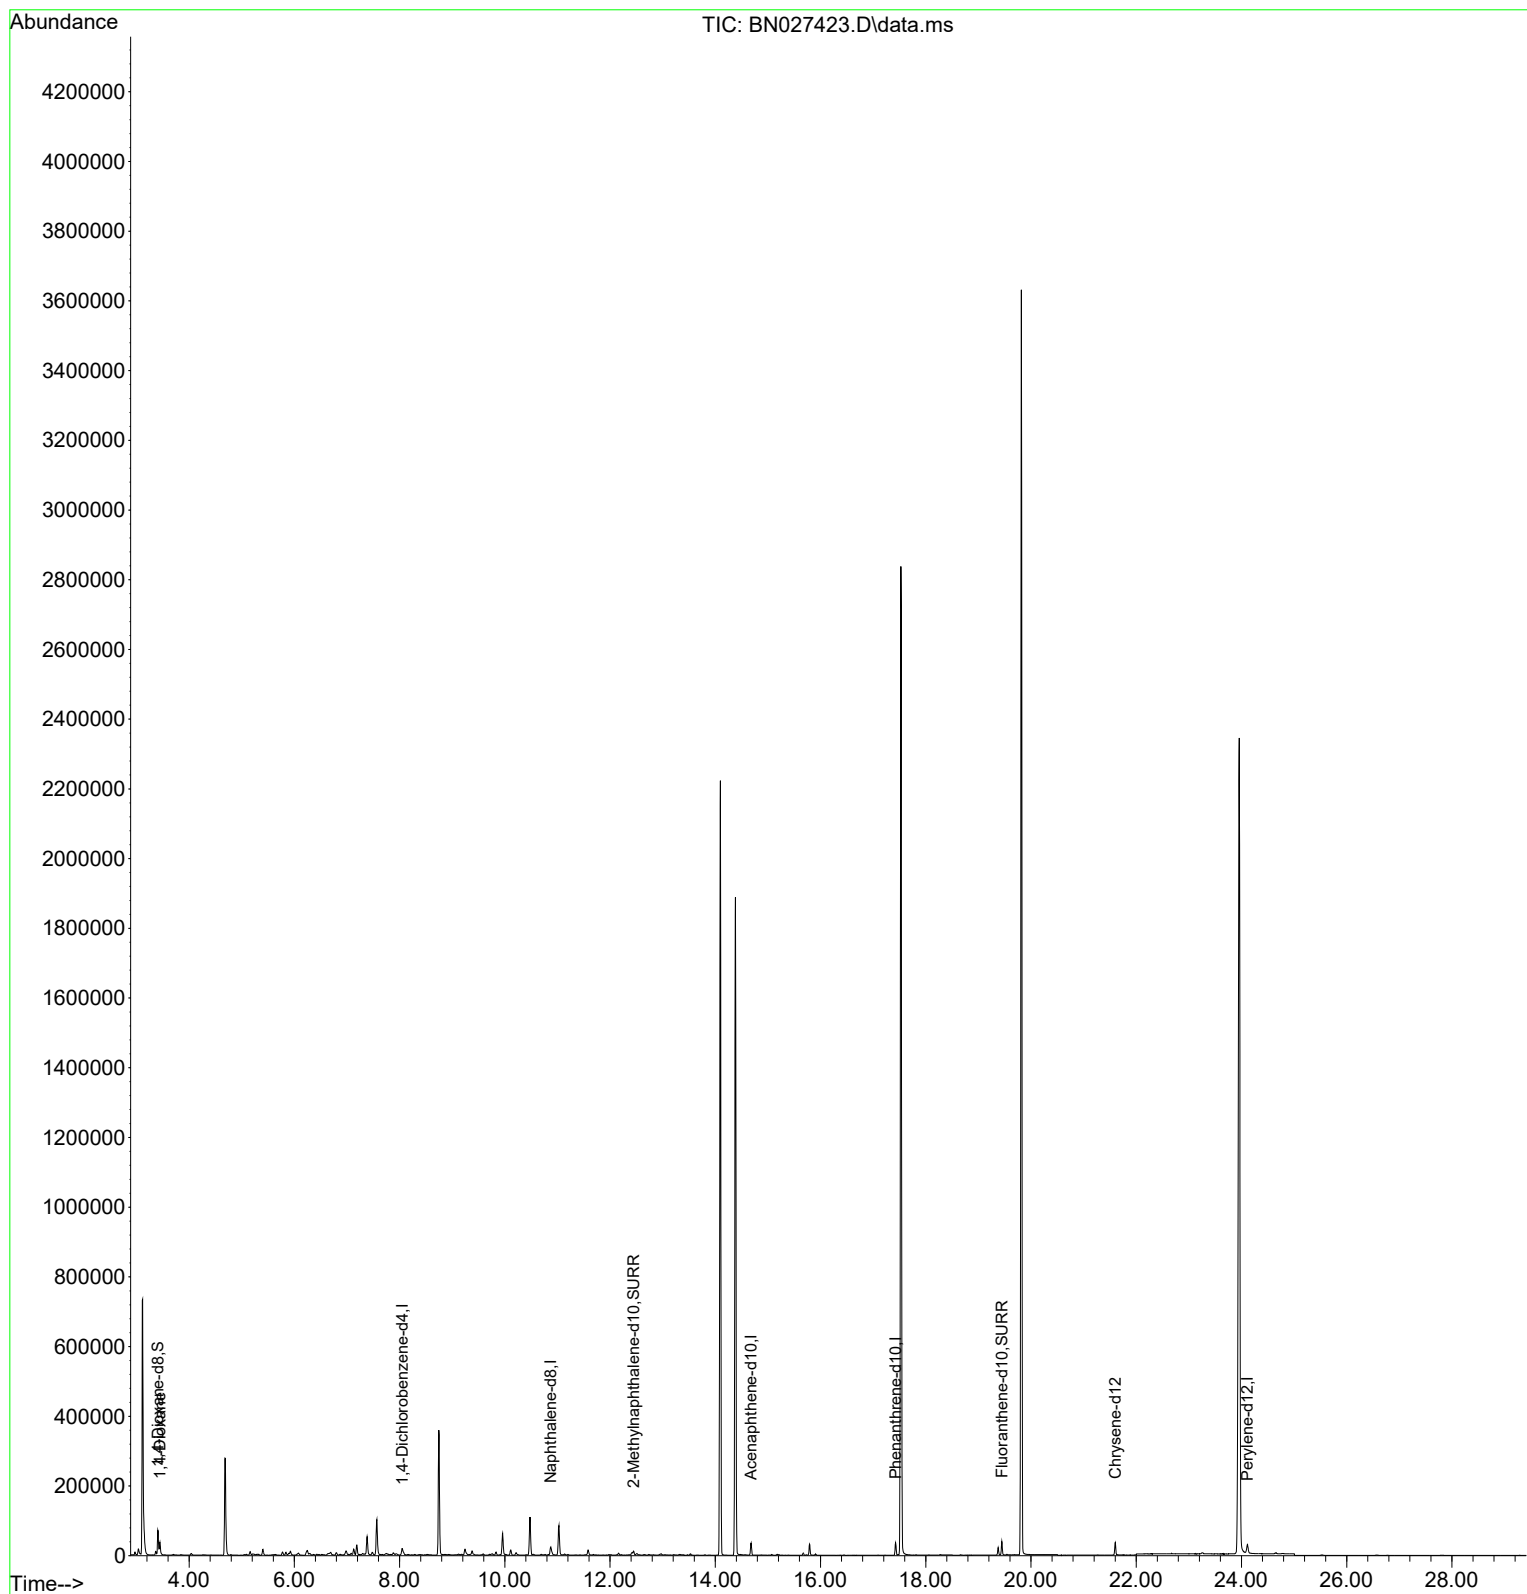

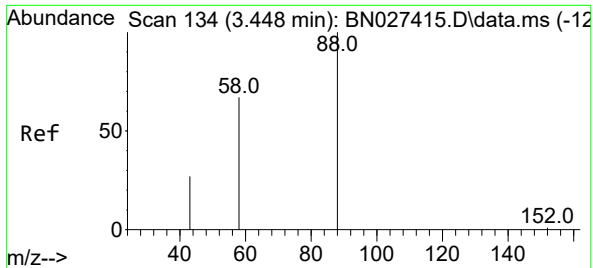

#2
1,4-Dioxane
Concen: 2.067 ng/ul
RT: 3.443 min Scan# 11
Delta R.T. -0.013 min
Lab File: BN027423.D
Acq: 07 Sep 2023 01:47

Instrument :
BNA_N
ClientSampleId :
BH942

Tgt Ion:	88	Resp:	24609
Ion	Ratio	Lower	Upper
88	100		
43	29.5	26.8	40.2
58	65.9	39.9	59.9

