

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027425.D
 Acq On : 07 Sep 2023 03:02
 Operator : MA/JU
 Sample : 04159-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHK7

Quant Time: Sep 07 04:38:14 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	6055	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.872	136	22103	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	13758	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	31080	0.400	ng/ul	-0.01
17) Chrysene-d12	21.597	240	23445	0.400	ng/ul	-0.01
23) Perylene-d12	24.108	264	23638	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	30308	3.763	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	12782	0.381	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	33511	0.417	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.054	266	19095	3.151	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027425.D
Acq On : 07 Sep 2023 03:02
Operator : MA/JU
Sample : 04159-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHK7


Quant Time: Sep 07 04:38:14 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

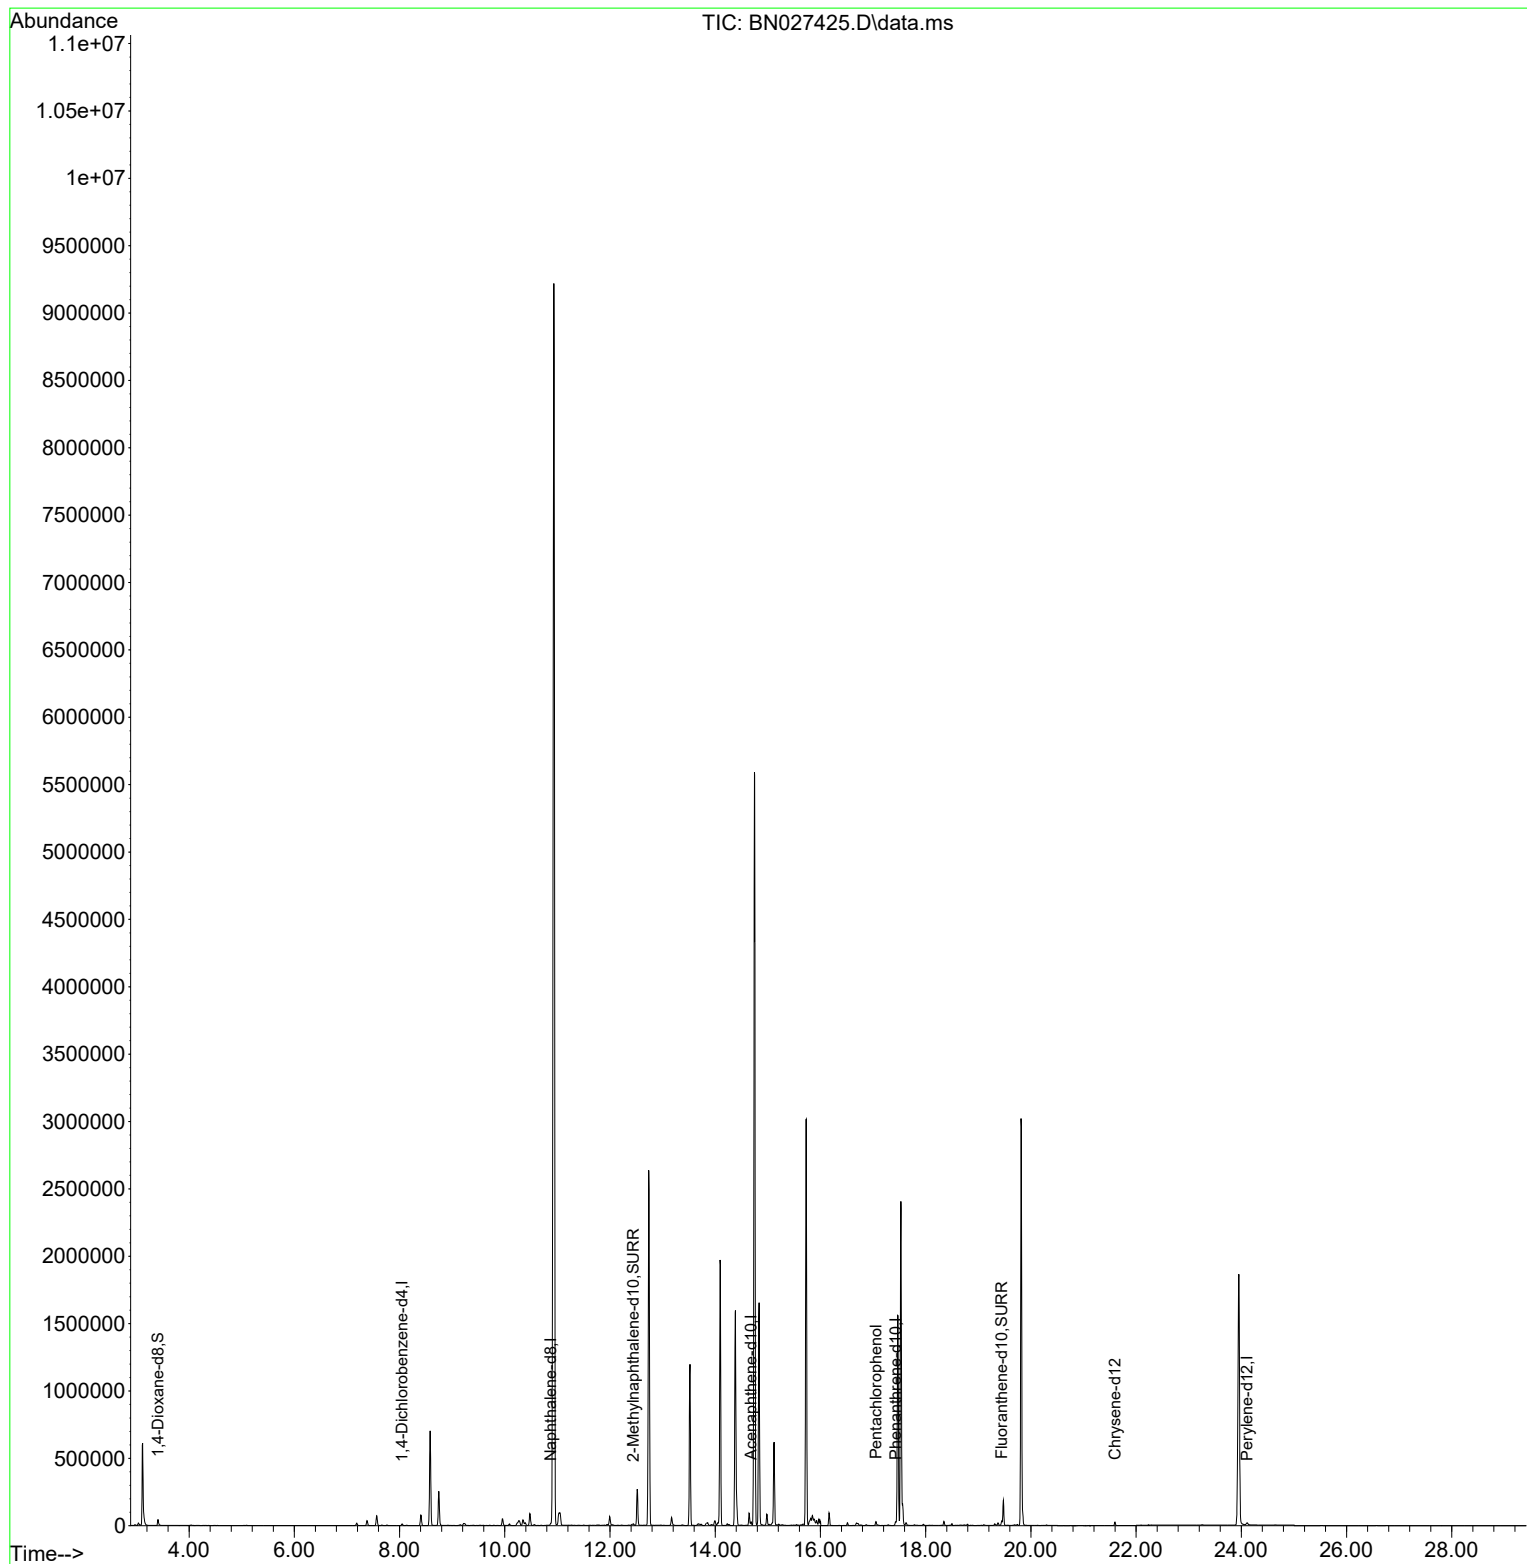

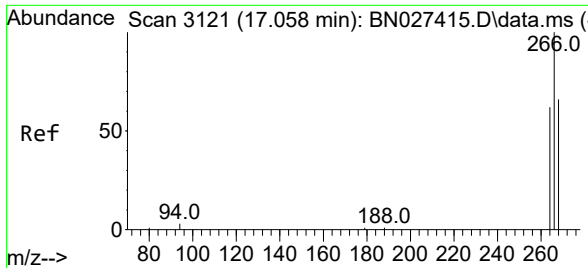

#14
Pentachlorophenol
Concen: 3.151 ng/ul
RT: 17.054 min Scan# 31
Delta R.T. -0.012 min
Lab File: BN027425.D
Acq: 07 Sep 2023 03:02

Instrument :
BNA_N
ClientSampleId :
DCHK7

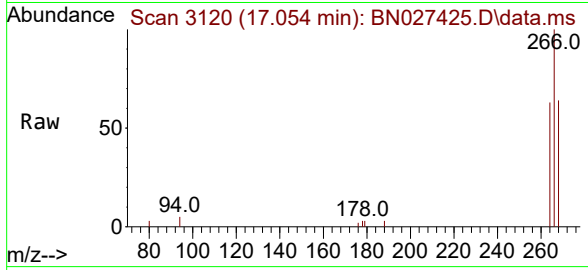

Tgt Ion:266 Resp: 19095
Ion Ratio Lower Upper
266 100
264 62.6 50.4 75.6
268 64.1 51.9 77.9

