

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027428.D
 Acq On : 07 Sep 2023 04:53
 Operator : MA/JU
 Sample : 04159-05DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHJ2DL

Quant Time: Sep 07 05:27:10 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	5310	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.872	136	17849	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	11378	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	26710	0.400	ng/ul	-0.01
17) Chrysene-d12	21.597	240	22131	0.400	ng/ul	-0.01
23) Perylene-d12	24.105	264	21625	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	2773	0.393	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	1807	0.067	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	5322	0.070	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	17.054	266	10693	2.053	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027428.D
Acq On : 07 Sep 2023 04:53
Operator : MA/JU
Sample : 04159-05DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHJ2DL

Quant Time: Sep 07 05:27:10 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

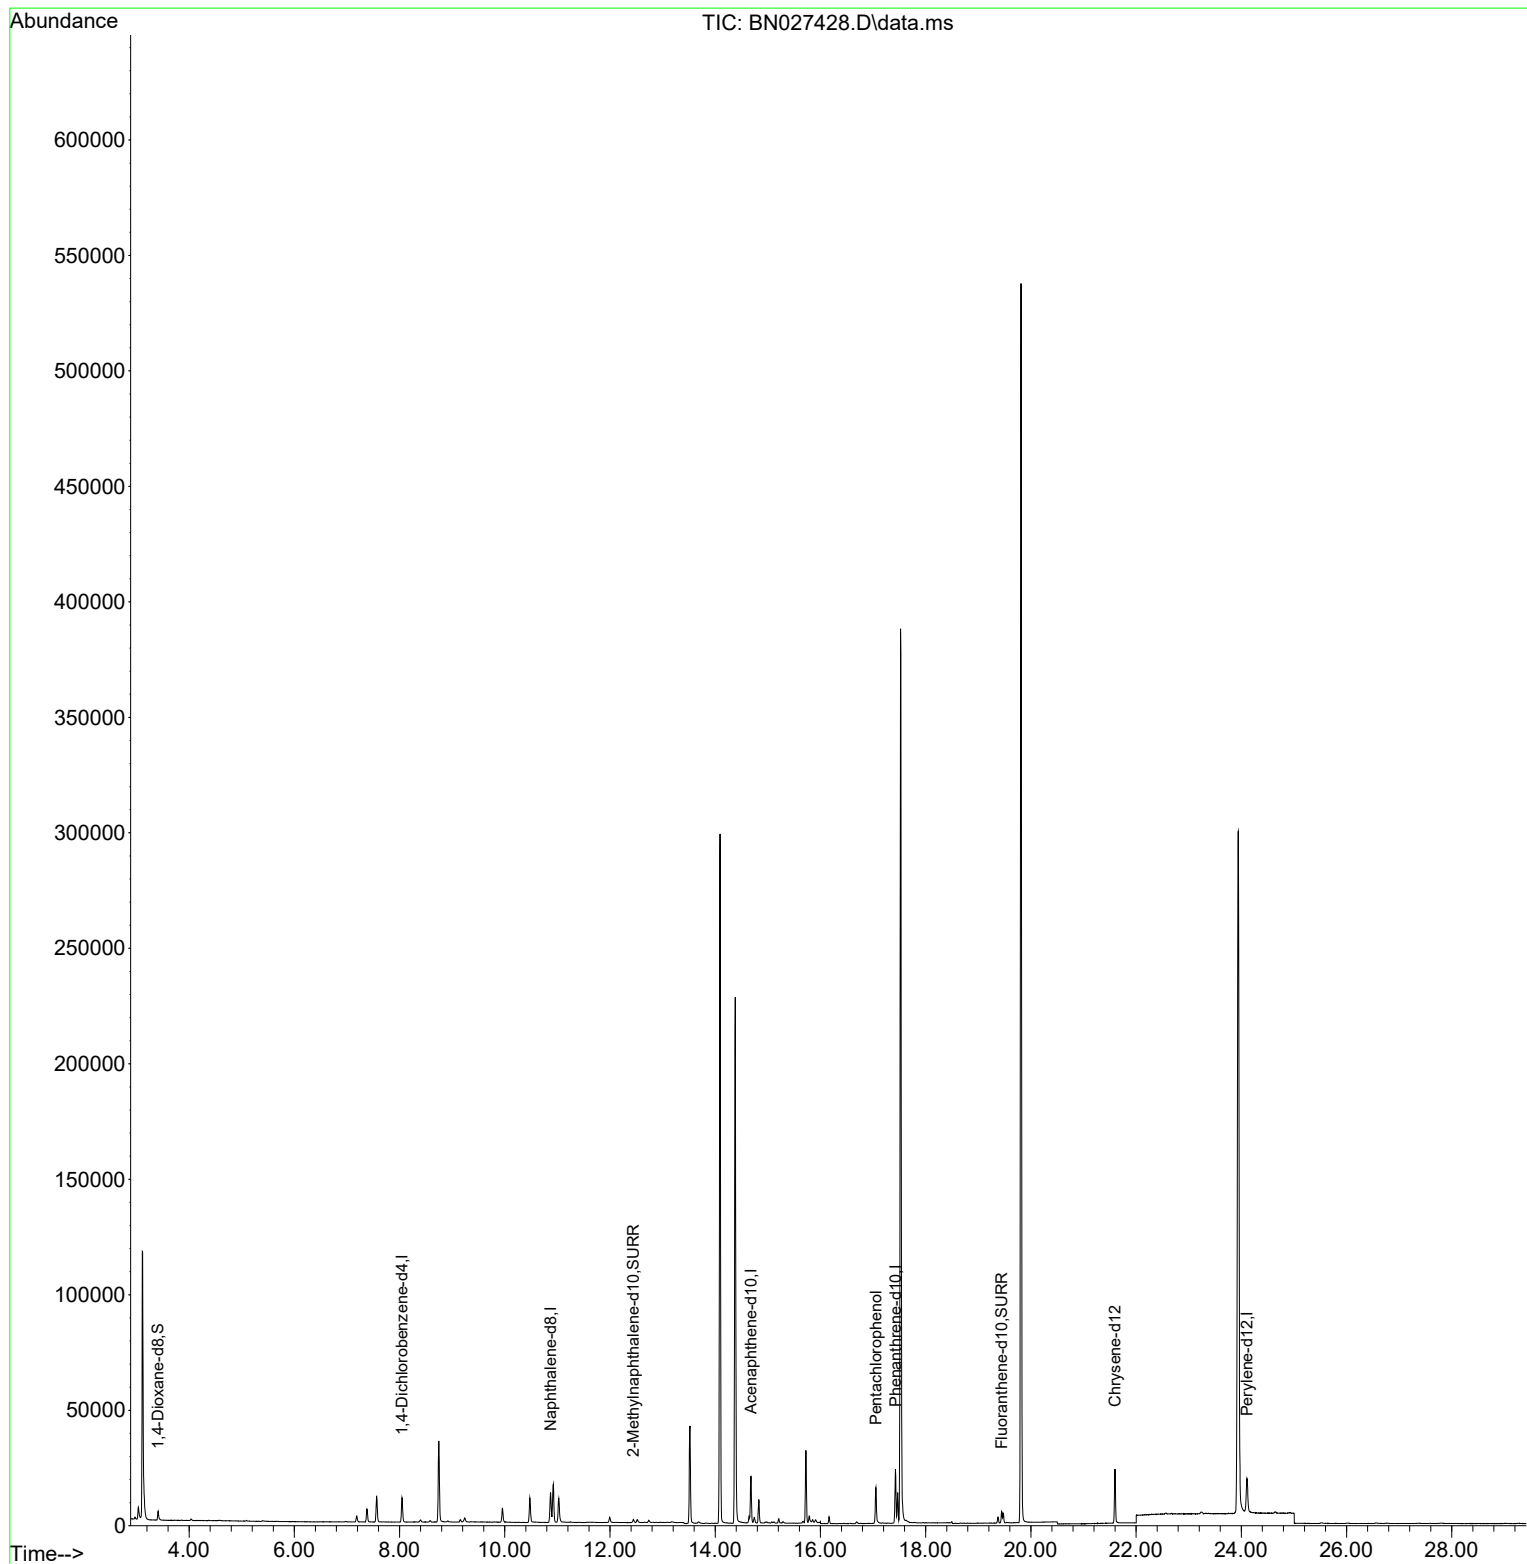

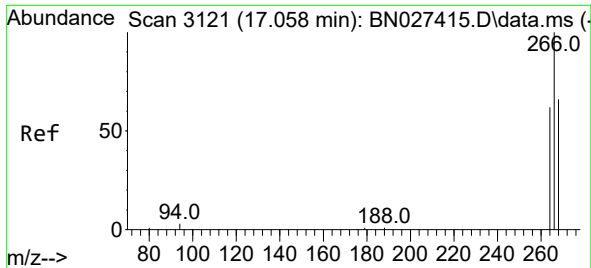

#14

Pentachlorophenol

Concen: 2.053 ng/ul

RT: 17.054 min Scan# 31

Delta R.T. -0.013 min

Lab File: BN027428.D


Acq: 07 Sep 2023 04:53

Instrument :

BNA_N

ClientSampleId :

DCHJ2DL

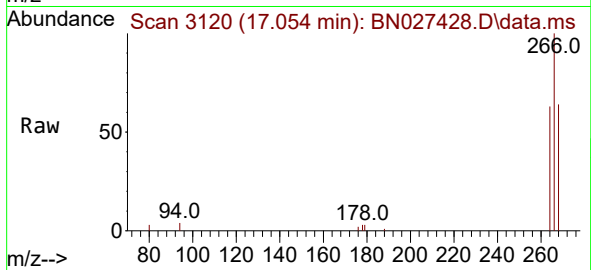

Tgt Ion:266 Resp: 10693

Ion Ratio Lower Upper

266 100

264 62.6 50.4 75.6

268 64.2 51.9 77.9

