

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027430.D
 Acq On : 07 Sep 2023 06:07
 Operator : MA/JU
 Sample : 04123-05
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHAA8

Quant Time: Sep 07 06:36:22 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	4800	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.867	136	17192	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.675	164	10979	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.426	188	24905	0.400	ng/ul	-0.01
17) Chrysene-d12	21.600	240	20129	0.400	ng/ul	0.00
23) Perylene-d12	24.108	264	20871	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	33821	5.297	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.445	152	9883	0.379	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	26466	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	647	0.100	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027430.D
Acq On : 07 Sep 2023 06:07
Operator : MA/JU
Sample : 04123-05
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHAA8

Quant Time: Sep 07 06:36:22 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

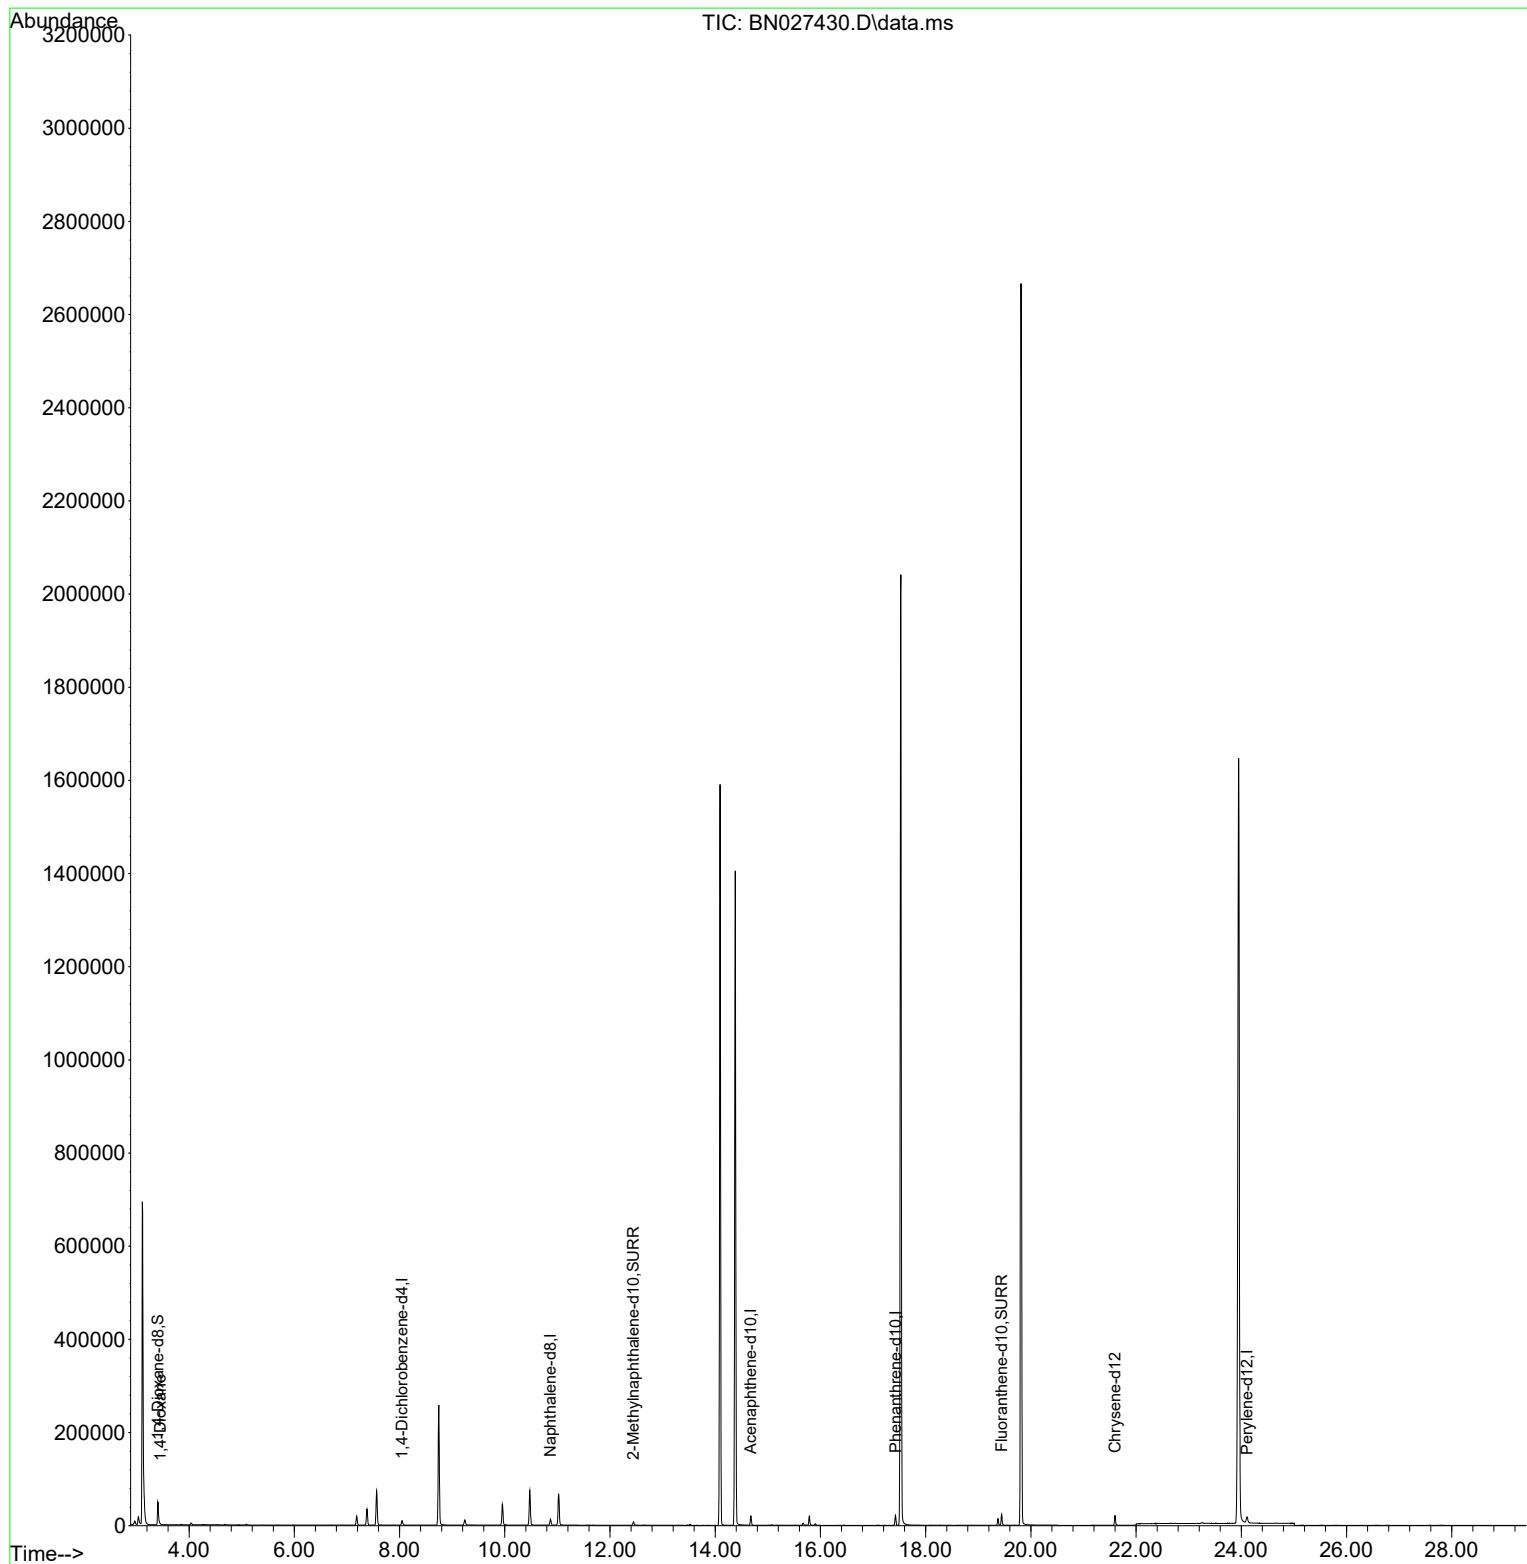

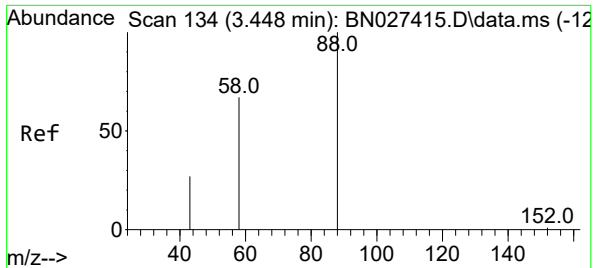

1,4-Dioxane
 Concen: 0.100 ng/ul
 RT: 3.448 min Scan# 11
 Delta R.T. -0.008 min
 Lab File: BN027430.D
 Acq: 07 Sep 2023 06:07

Instrument :
 BNA_N
 ClientSampleId :
 BHAA8

Tgt Ion:	88	Resp:	647
Ion	Ratio	Lower	Upper
88	100		
43	64.7	26.8	40.2#
58	45.6	39.9	59.9

