

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027441.D
 Acq On : 07 Sep 2023 14:09
 Operator : MA/JU
 Sample : 04123-02
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH923

Quant Time: Sep 08 01:56:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	8567	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	28860	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.684	164	16382	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.434	188	33679	0.400	ng/ul	0.00
17) Chrysene-d12	21.615	240	21362	0.400	ng/ul	# 0.00
23) Perylene-d12	24.132	264	21155	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	44924	3.942	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.451	152	13703	0.313	ng/ul	0.00
18) Fluoranthene-d10	19.455	212	29042	0.397	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	1812	0.157	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027441.D
Acq On : 07 Sep 2023 14:09
Operator : MA/JU
Sample : 04123-02
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH923

Quant Time: Sep 08 01:56:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

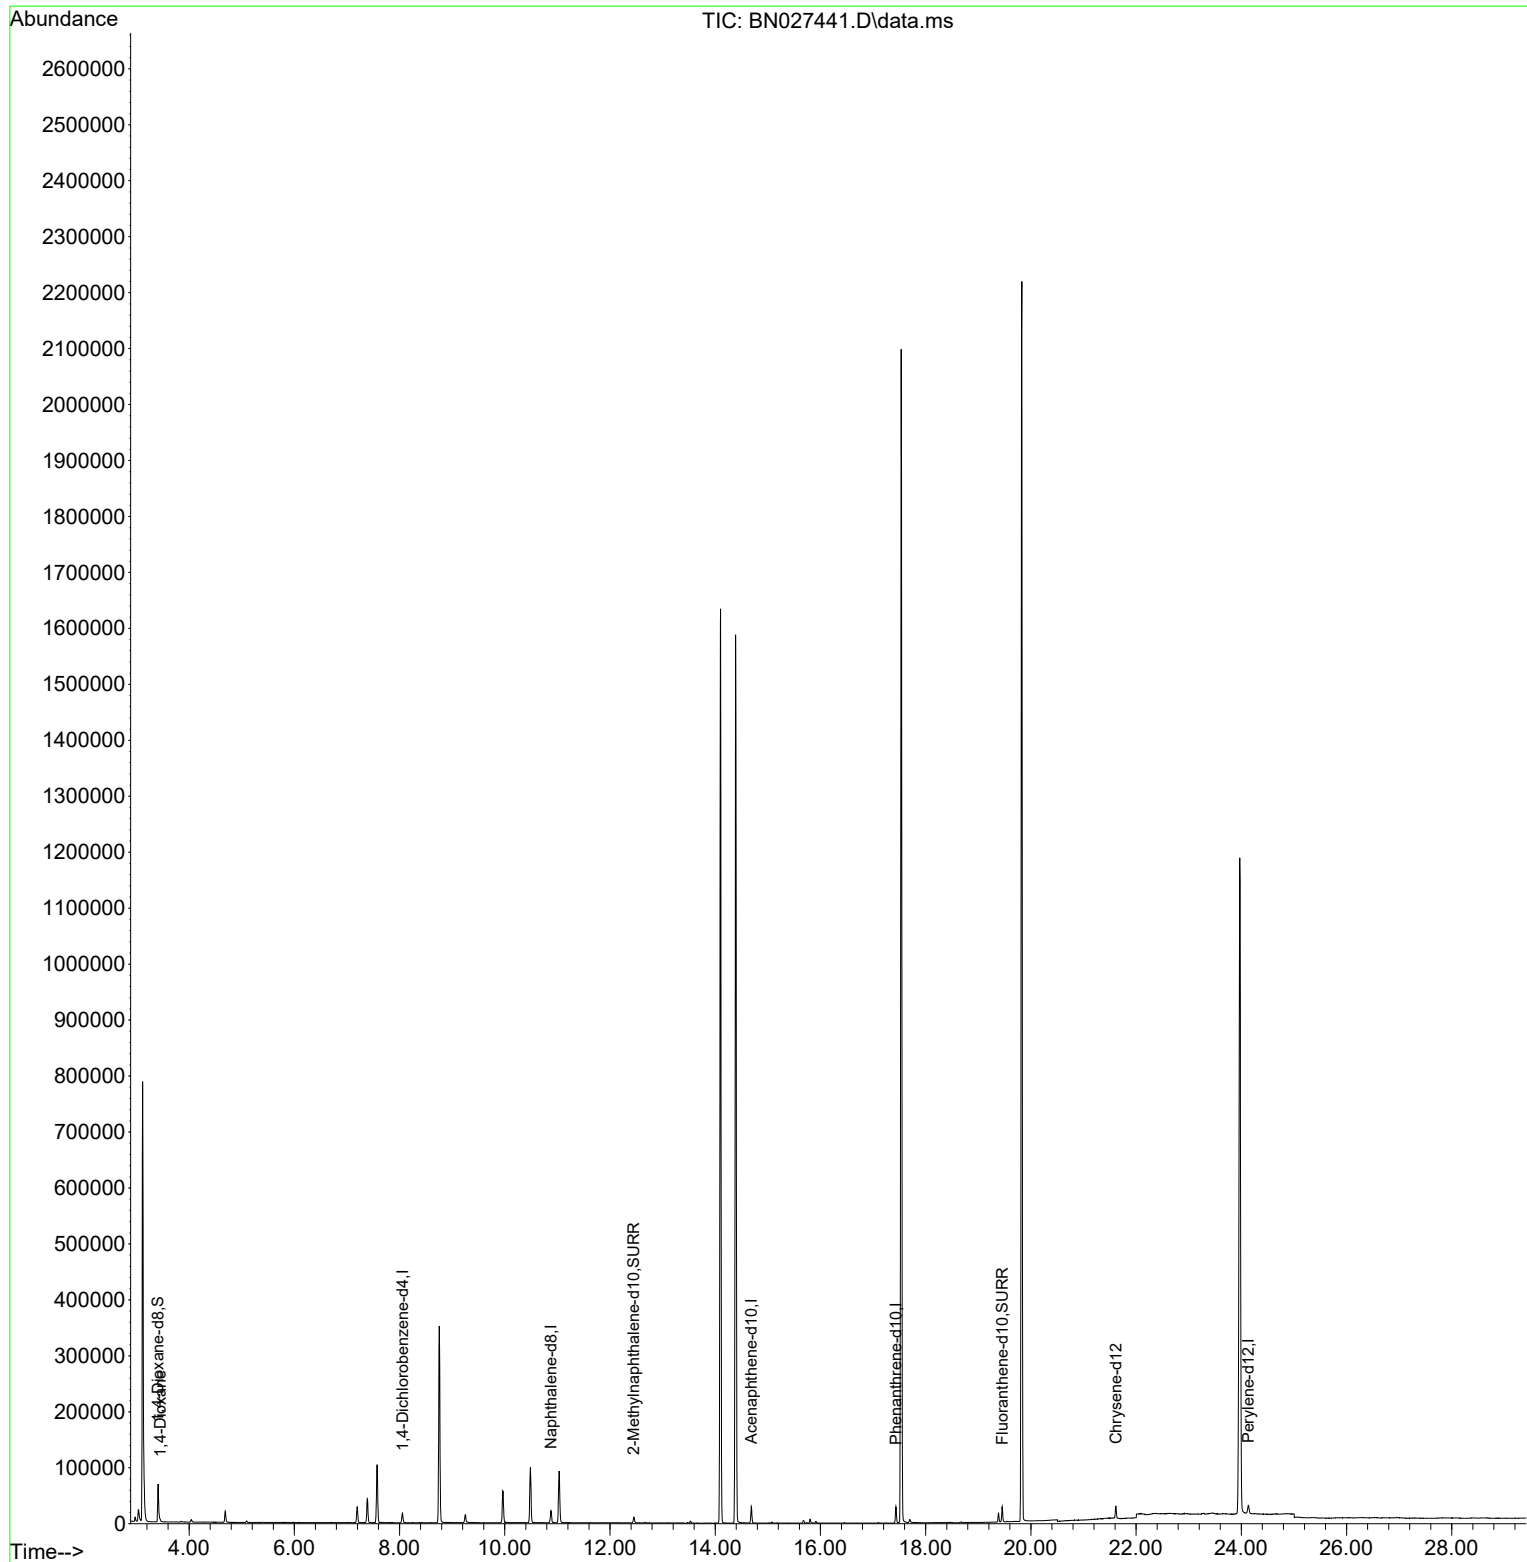

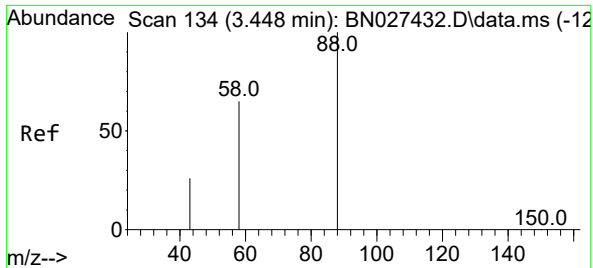

1,4-Dioxane
 Concen: 0.157 ng/ul
 RT: 3.448 min Scan# 11
 Delta R.T. -0.009 min
 Lab File: BN027441.D
 Acq: 07 Sep 2023 14:09

Instrument :
 BNA_N
 ClientSampleId :
 BH923

Tgt Ion: 88 Resp: 1812
 Ion Ratio Lower Upper
 88 100
 43 74.7 26.8 40.2#
 58 58.5 39.9 59.9

