

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027456.D
 Acq On : 08 Sep 2023 00:16
 Operator : MA/JU
 Sample : 04123-17
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9F9

Quant Time: Sep 08 01:58:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 02 06:16:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	7820	0.400	ng/ul	0.00
4) Naphthalene-d8	10.872	136	26743	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.680	164	15755	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.430	188	33645	0.400	ng/ul	0.00
17) Chrysene-d12	21.600	240	22299	0.400	ng/ul	0.00
23) Perylene-d12	24.108	264	22210	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	54492	5.238	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	16708	0.412	ng/ul	-0.01
18) Fluoranthene-d10	19.445	212	38757	0.507	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	1684	0.160	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027456.D
Acq On : 08 Sep 2023 00:16
Operator : MA/JU
Sample : 04123-17
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9F9

Quant Time: Sep 08 01:58:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 02 06:16:48 2023
Response via : Initial Calibration

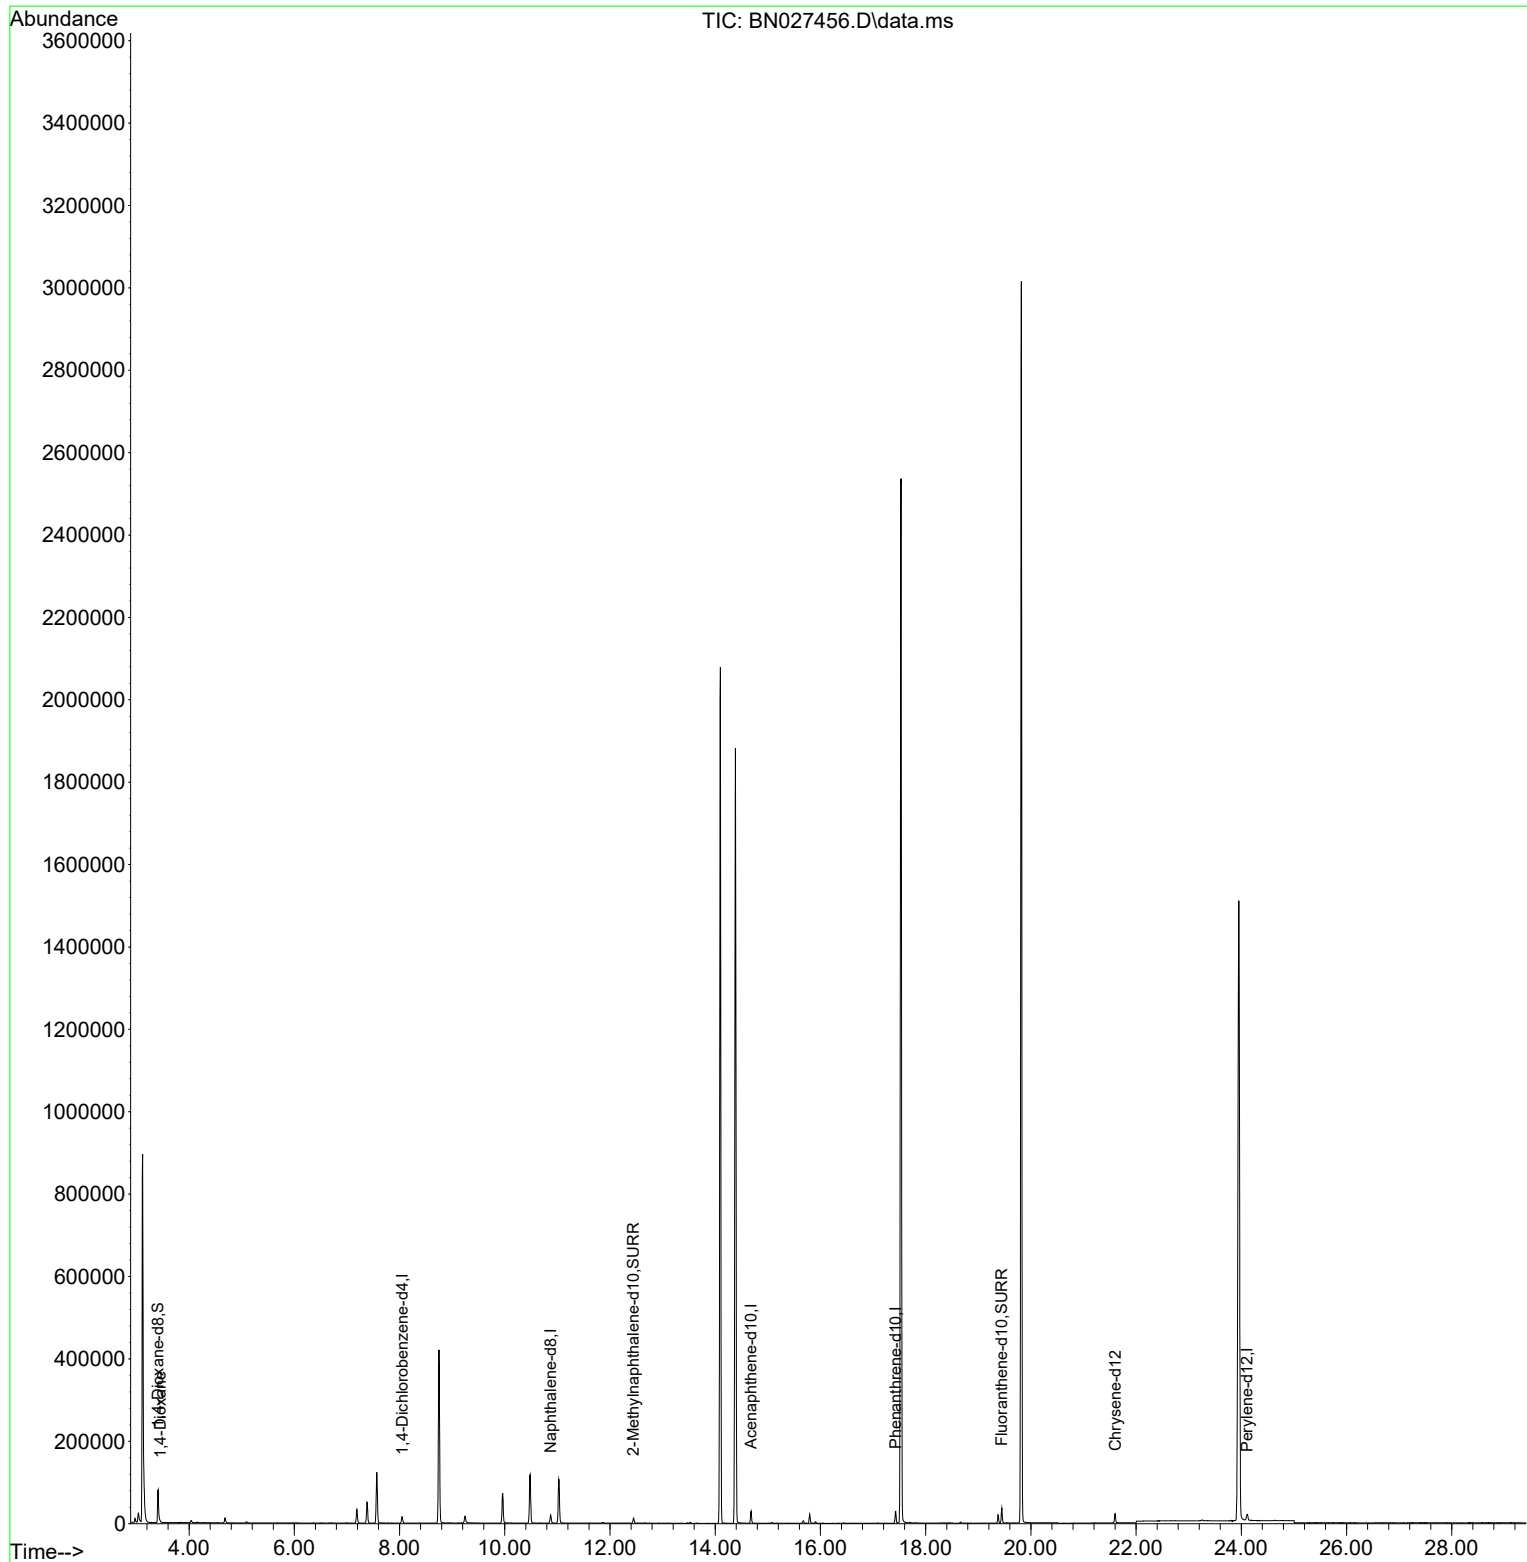

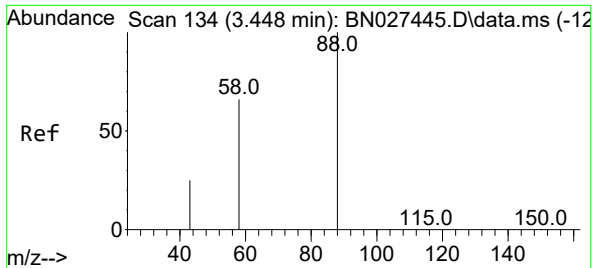

#2
 1,4-Dioxane
 Concen: 0.160 ng/ul
 RT: 3.448 min Scan# 11
 Delta R.T. -0.009 min
 Lab File: BN027456.D
 Acq: 08 Sep 2023 00:16

Instrument :
 BNA_N
 ClientSampleId :
 BH9F9

Tgt Ion: 88 Resp: 1684
 Ion Ratio Lower Upper
 88 100
 43 58.7 26.8 40.2#
 58 54.3 39.9 59.9

