

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027465.D
 Acq On : 08 Sep 2023 06:27
 Operator : MA/JU
 Sample : 04166-09
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKJ9

Quant Time: Sep 08 06:56:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	7566	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	26369	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.680	164	17065	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	34595	0.400	ng/ul	0.00
17) Chrysene-d12	21.597	240	22604	0.400	ng/ul	0.00
23) Perylene-d12	24.109	264	21332	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	42421	4.215	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	15925	0.398	ng/ul	0.00
18) Fluoranthene-d10	19.446	212	38352	0.495	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.443	88	17373	1.706	ng/ul#	86
5) Naphthalene	10.922	128	2469	0.032	ng/ul#	48
14) Pentachlorophenol	17.054	266	15588	2.311	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027465.D
Acq On : 08 Sep 2023 06:27
Operator : MA/JU
Sample : 04166-09
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKJ9

Quant Time: Sep 08 06:56:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




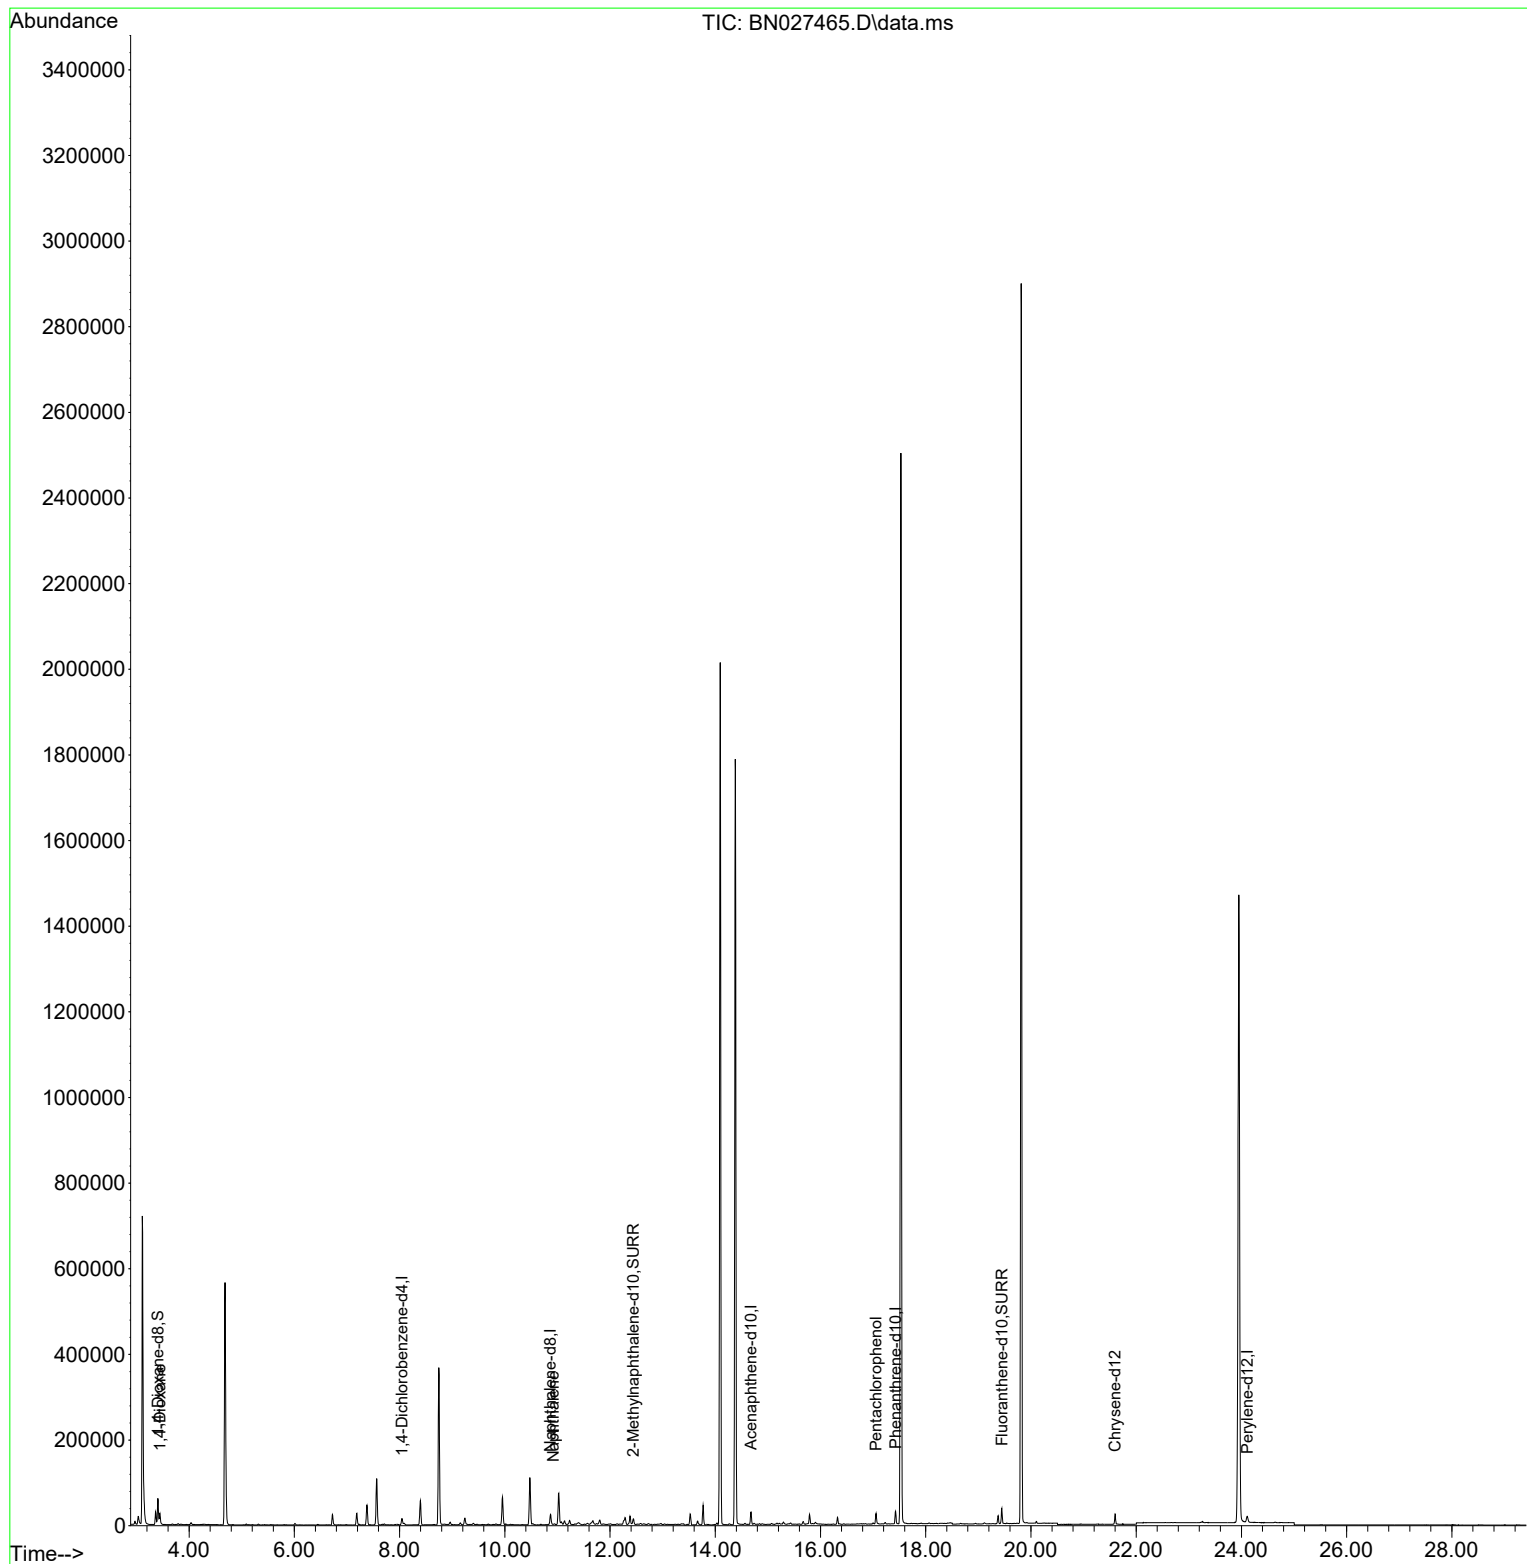


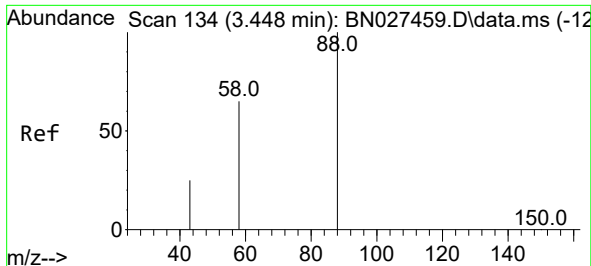

#2
1,4-Dioxane
Concen: 1.706 ng/ul
RT: 3.443 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027465.D
Acq: 08 Sep 2023 06:27




Instrument :
BNA_N
ClientSampleId :
BBKJ9


Tgt Ion: 88 Resp: 17373
Ion Ratio Lower Upper
88 100
43 31.2 26.8 40.2
58 64.0 39.9 59.9#

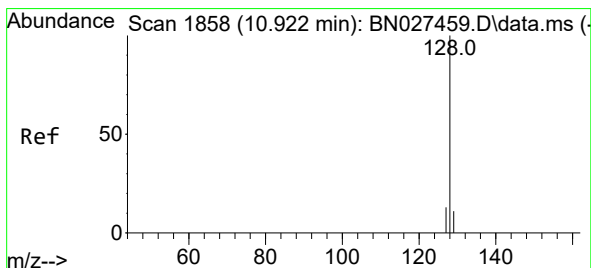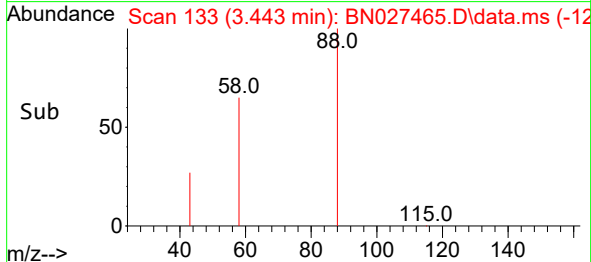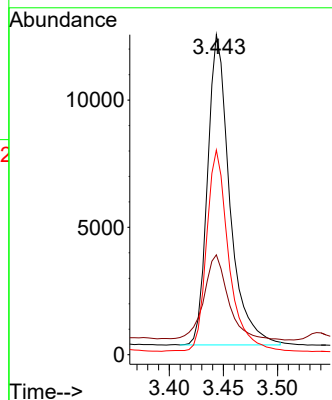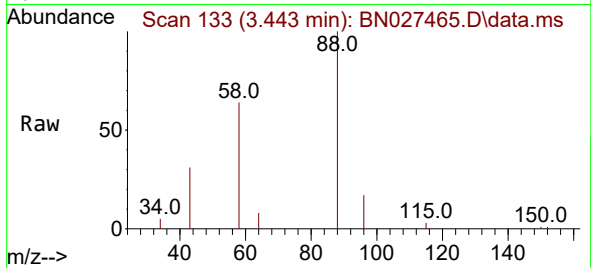

#5
Naphthalene
Concen: 0.032 ng/ul
RT: 10.922 min Scan# 1858
Delta R.T. -0.000 min
Lab File: BN027465.D
Acq: 08 Sep 2023 06:27


Tgt Ion: 128 Resp: 2469
Ion Ratio Lower Upper
128 100
129 37.5 9.4 14.0#
127 29.0 10.6 16.0#

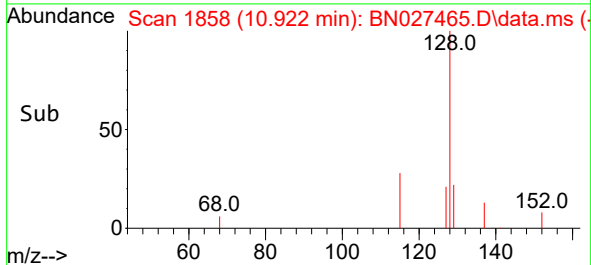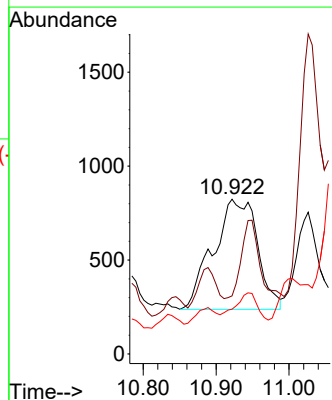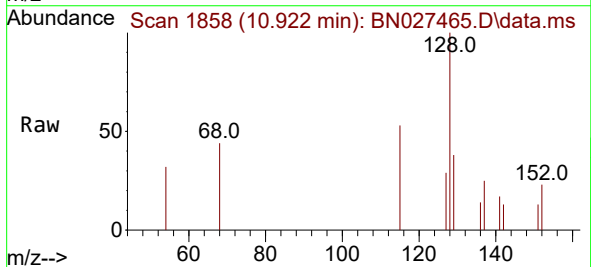

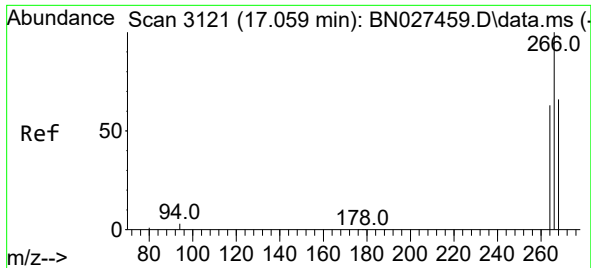

#14
Pentachlorophenol
Concen: 2.311 ng/ul
RT: 17.054 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN027465.D
Acq: 08 Sep 2023 06:27

Instrument :
BNA_N
ClientSampleId :
BBKJ9

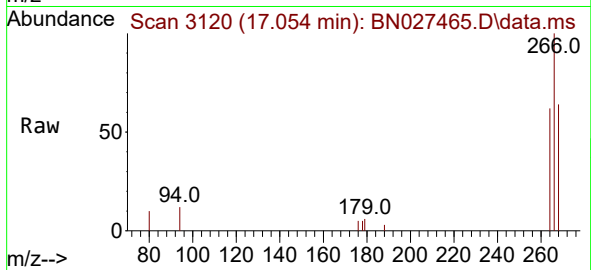

Tgt Ion:266 Resp: 15588
Ion Ratio Lower Upper
266 100
264 63.0 50.4 75.6
268 64.2 51.9 77.9

