

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027468.D
 Acq On : 08 Sep 2023 08:17
 Operator : MA/JU
 Sample : 04166-12
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBK13

Quant Time: Sep 08 08:50:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	8004	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	27890	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.680	164	16548	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	34626	0.400	ng/ul	0.00
17) Chrysene-d12	21.603	240	22497	0.400	ng/ul	0.00
23) Perylene-d12	24.114	264	21706	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	40950	3.846	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	14490	0.342	ng/ul	0.00
18) Fluoranthene-d10	19.445	212	34682	0.450	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	24719	2.294	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027468.D
Acq On : 08 Sep 2023 08:17
Operator : MA/JU
Sample : 04166-12
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBK13

Quant Time: Sep 08 08:50:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

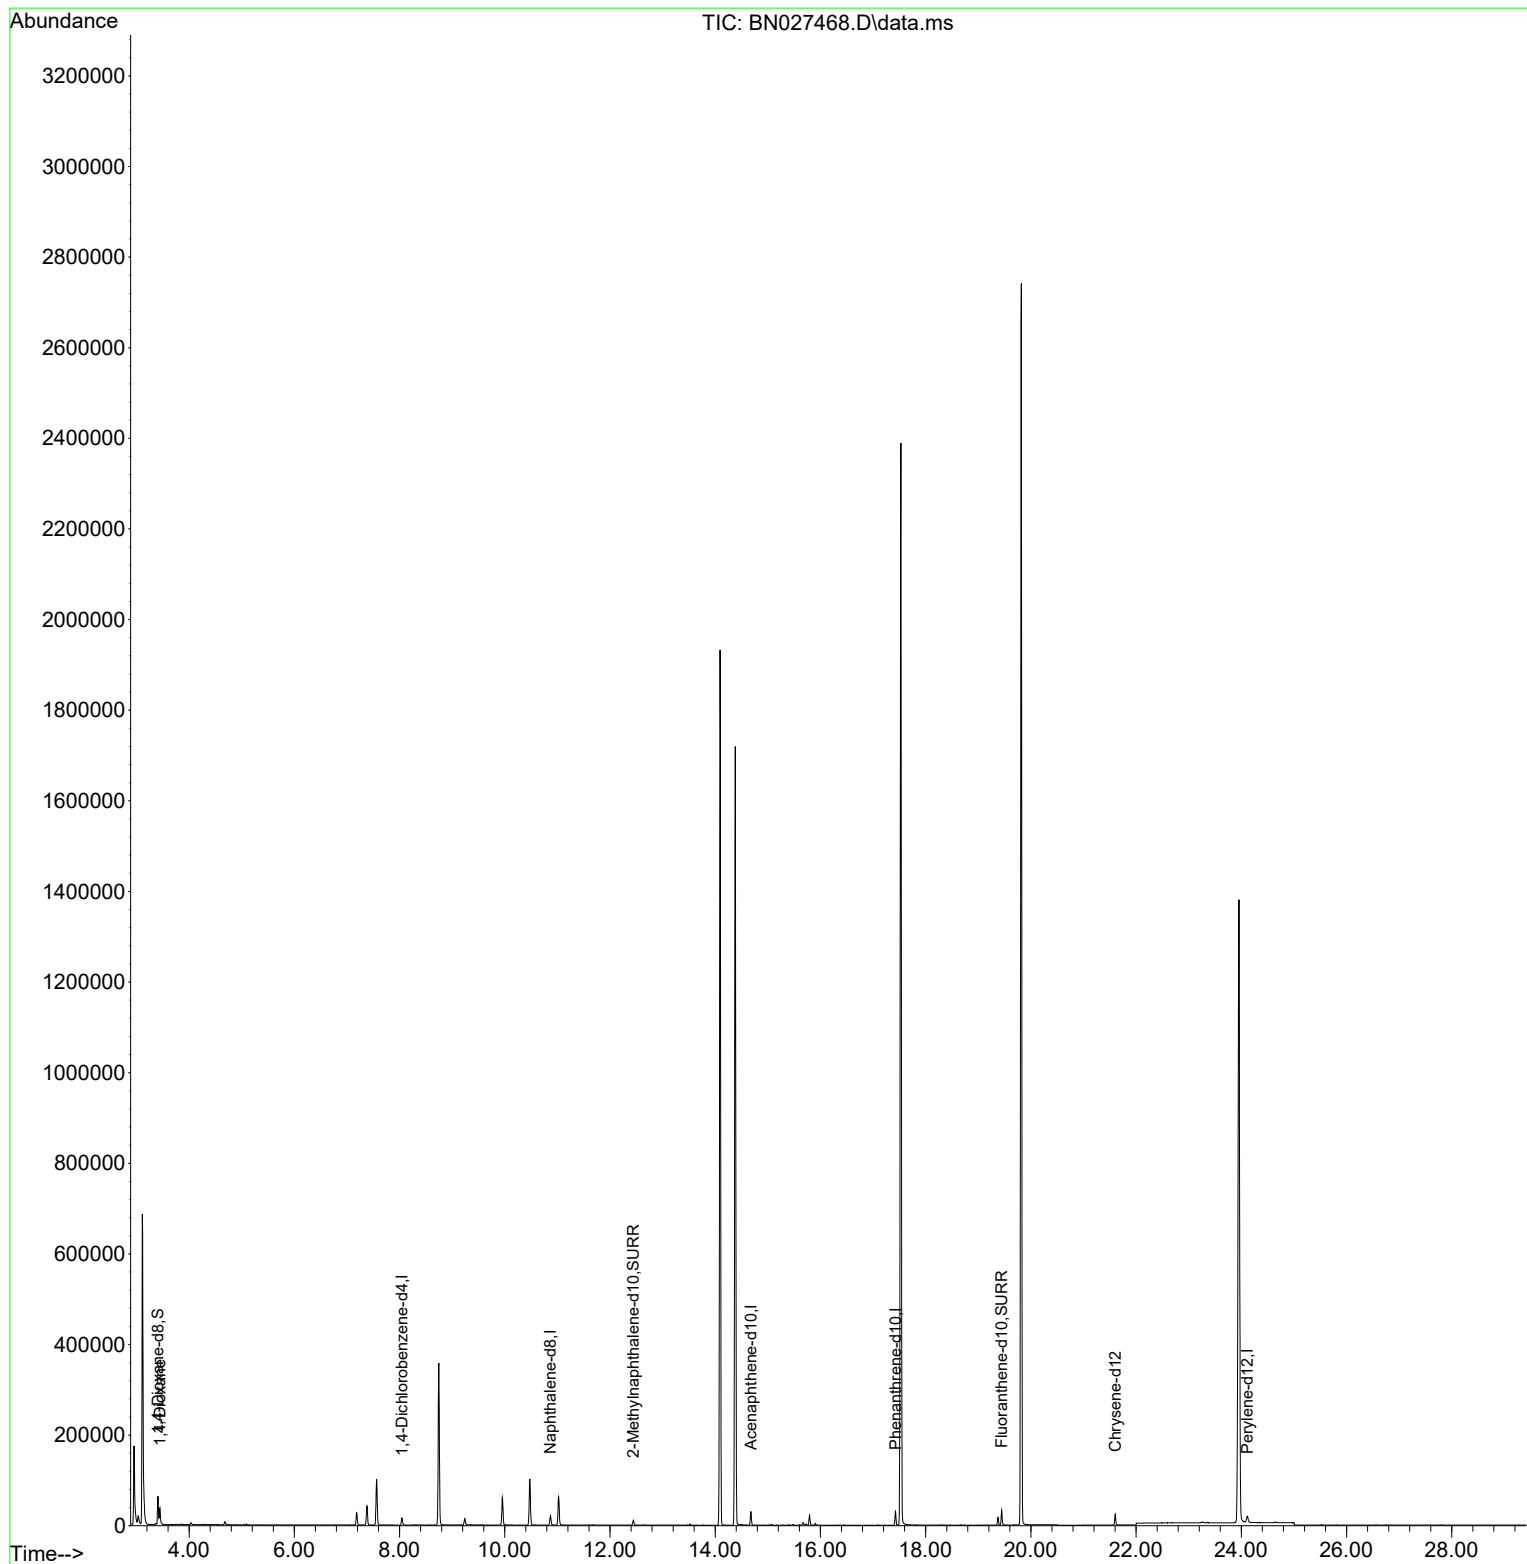

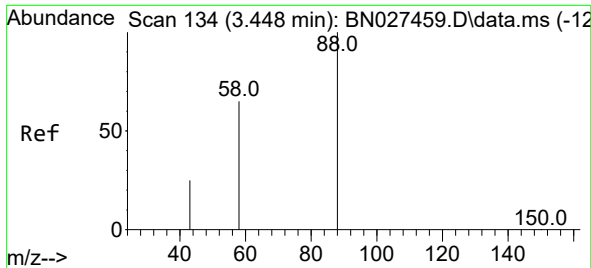

1,4-Dioxane

Concen: 2.294 ng/ul

RT: 3.444 min Scan# 11

Delta R.T. -0.004 min

Lab File: BN027468.D


Acq: 08 Sep 2023 08:17

Instrument :

BNA_N

ClientSampleId :

BBK13

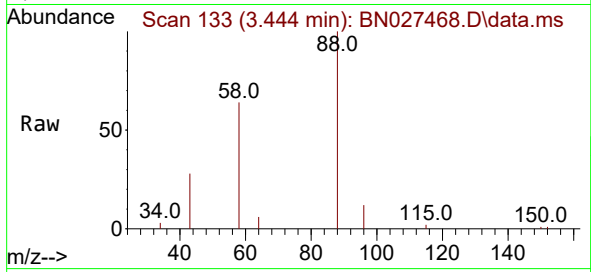

Tgt Ion: 88 Resp: 24719

Ion Ratio Lower Upper

88 100

43 27.8 26.8 40.2

58 64.2 39.9 59.9#

