

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
 Data File : BN027469.D
 Acq On : 08 Sep 2023 08:54
 Operator : MA/JU
 Sample : 04166-13
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHH3

Quant Time: Sep 09 00:07:28 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	7317	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	25387	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.675	164	15042	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	31595	0.400	ng/ul	0.00
17) Chrysene-d12	21.600	240	20045	0.400	ng/ul	0.00
23) Perylene-d12	24.108	264	19469	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	37017	3.803	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	13441	0.349	ng/ul	0.00
18) Fluoranthene-d10	19.445	212	31559	0.460	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	2173	0.221	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090623\
Data File : BN027469.D
Acq On : 08 Sep 2023 08:54
Operator : MA/JU
Sample : 04166-13
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHH3


Quant Time: Sep 09 00:07:28 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

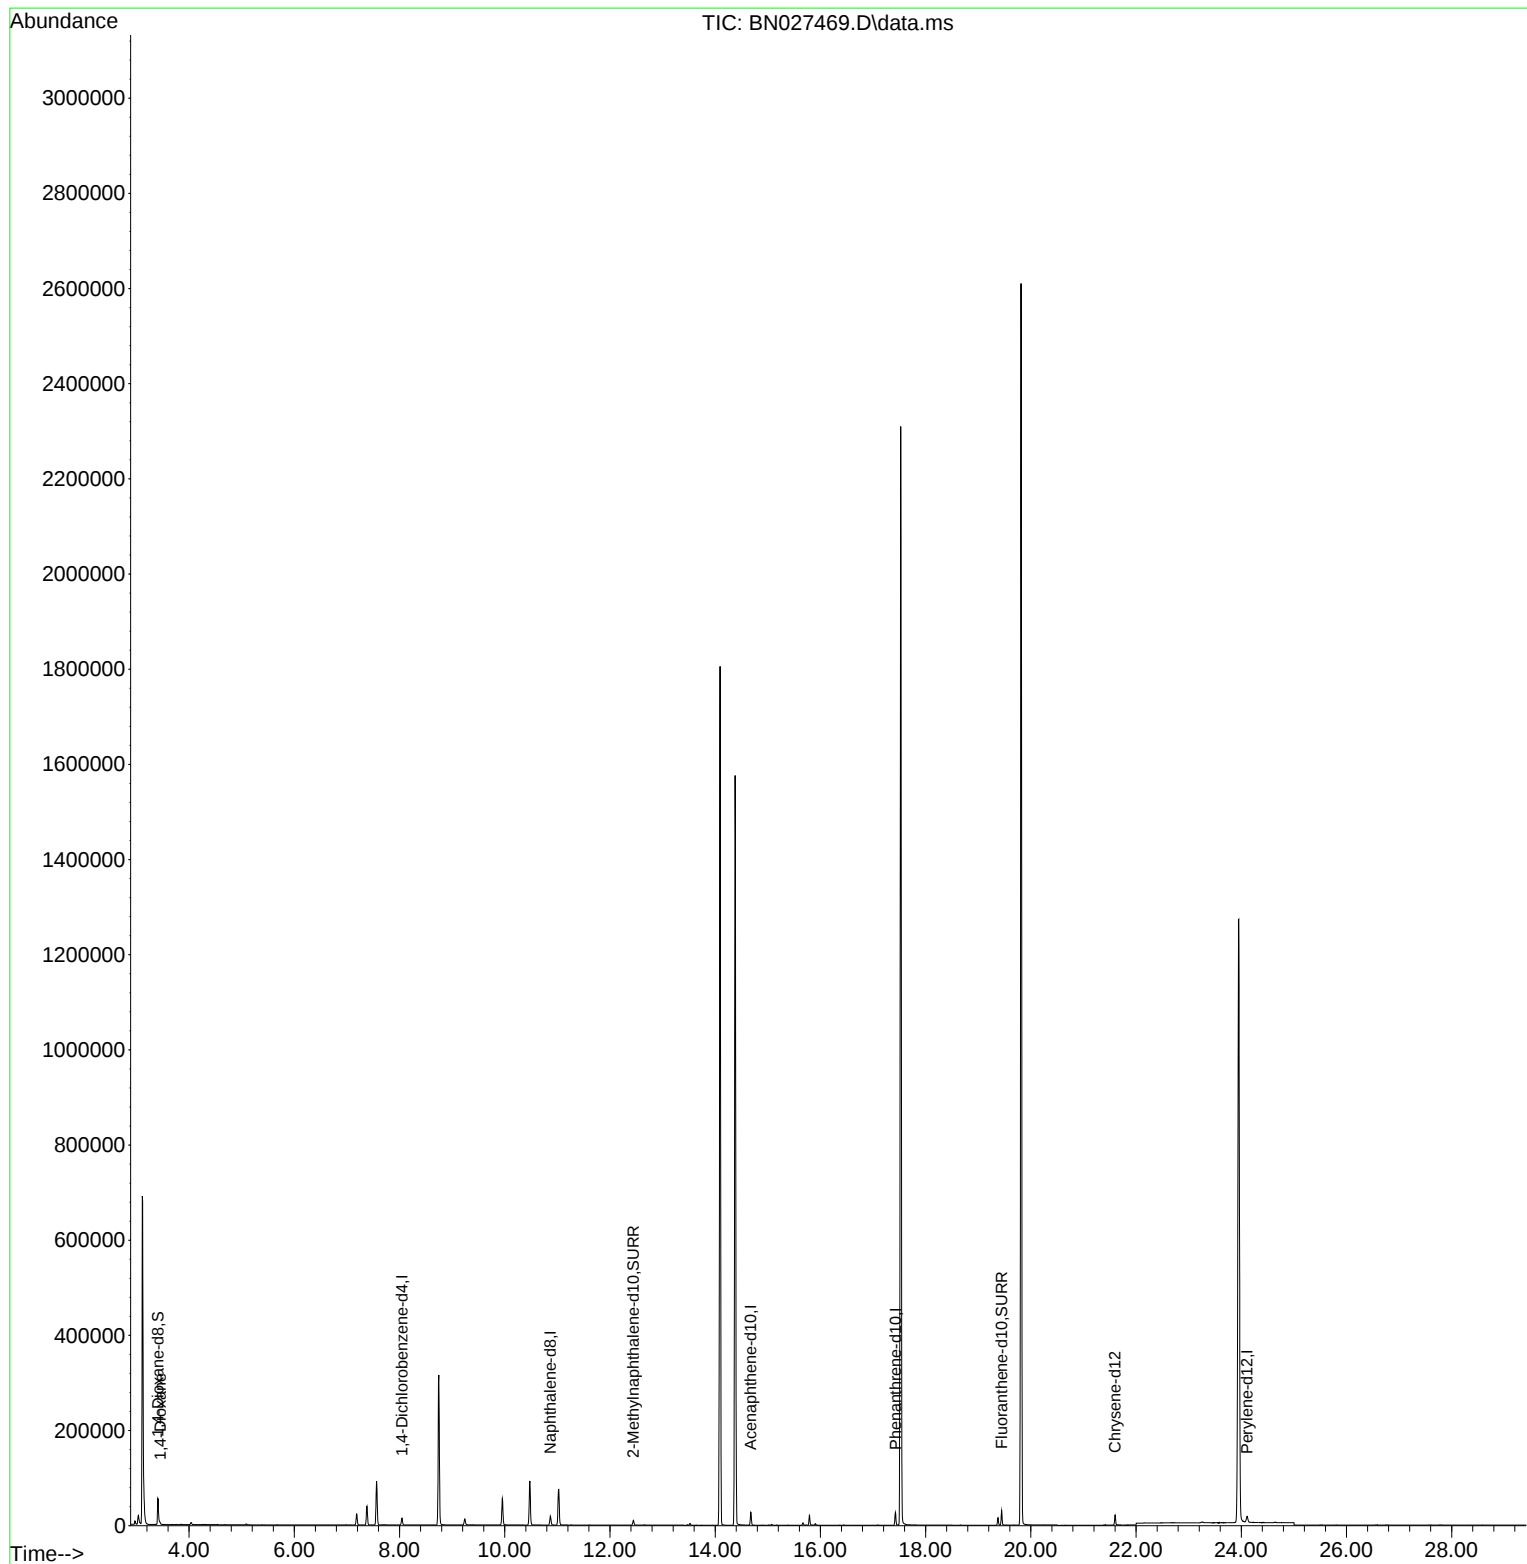

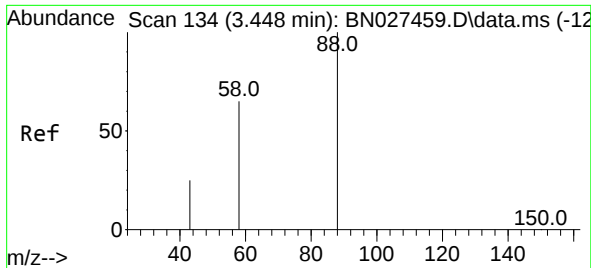

#2
1,4-Dioxane
Concen: 0.221 ng/ul
RT: 3.448 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN027469.D
Acq: 08 Sep 2023 08:54

Instrument :
BNA_N
ClientSampleId :
BBHH3

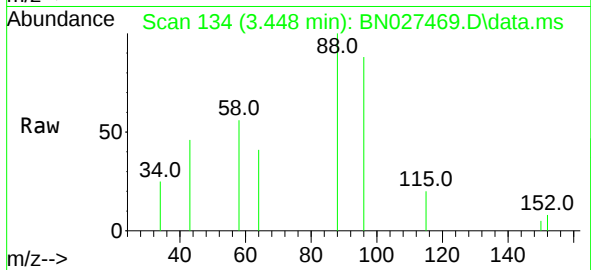

Tgt Ion: 88 Resp: 2173

Ion	Ratio	Lower	Upper
88	100		
43	46.3	26.8	40.2#
58	56.2	39.9	59.9

