

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090823\
 Data File : BN027479.D
 Acq On : 08 Sep 2023 16:57
 Operator : MA/JU
 Sample : PB155273BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 09 00:27:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.047	152	5425	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	18335	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.675	164	11682	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	26656	0.400	ng/ul	0.00
17) Chrysene-d12	21.598	240	22366	0.400	ng/ul	0.00
23) Perylene-d12	24.106	264	23236	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	36702	5.086	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	7864	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.446	212	20971	0.274	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.670	166	2967	0.058	ng/ul#	14
20) Pyrene	19.813	202	3093	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.942	252	6502	0.076	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090823\
Data File : BN027479.D
Acq On : 08 Sep 2023 16:57
Operator : MA/JU
Sample : PB155273BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Sep 09 00:27:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

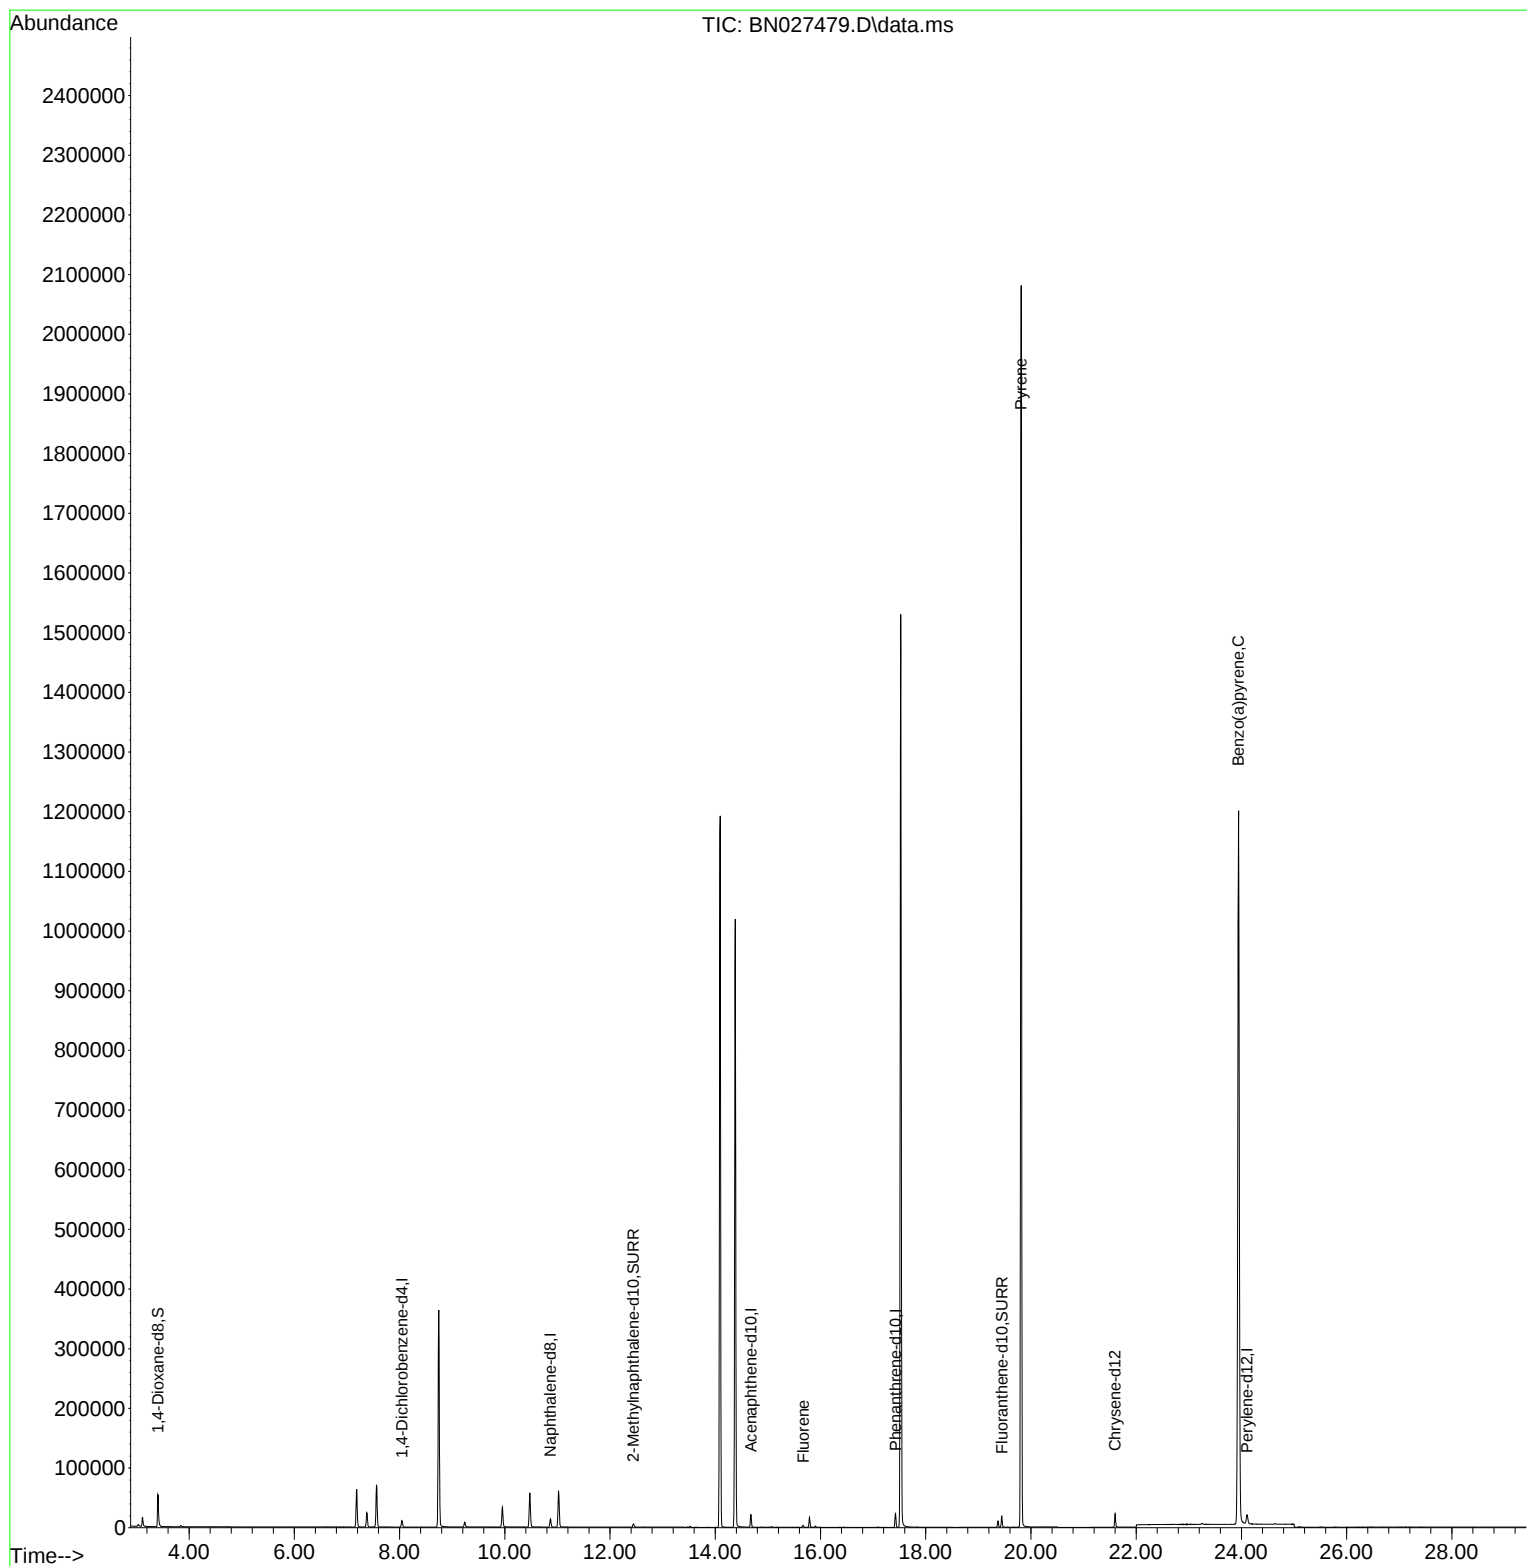



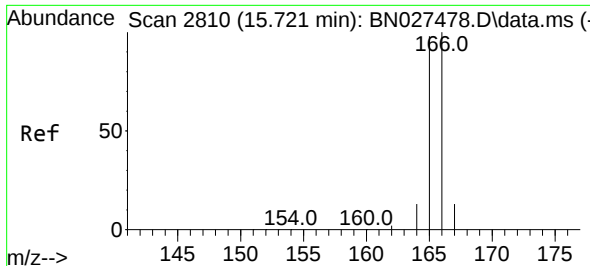


#12
Fluorene
Concen: 0.058 ng/ul
RT: 15.670 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN027479.D
Acq: 08 Sep 2023 16:57

Instrument :
BNA_N
ClientSampleId :



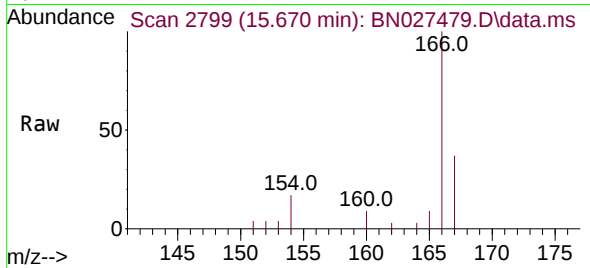



Tgt Ion:166 Resp: 2967
Ion Ratio Lower Upper
166 100
165 9.0 79.6 119.4#
167 36.8 11.4 17.0#

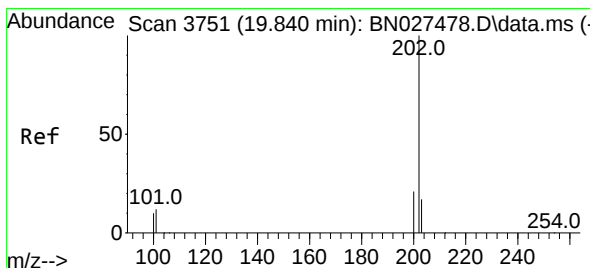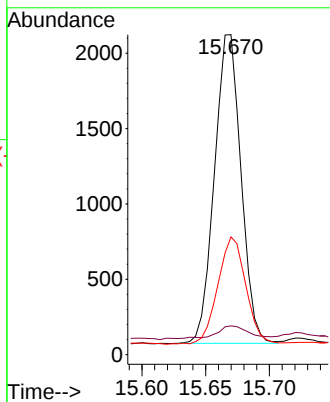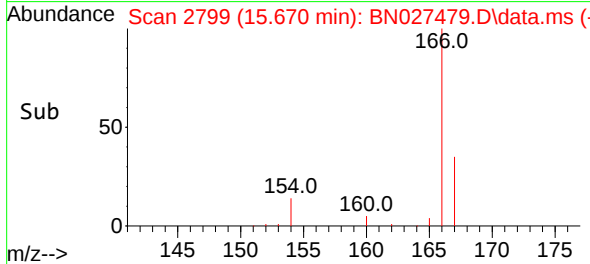

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.813 min Scan# 3745
Delta R.T. -0.028 min
Lab File: BN027479.D
Acq: 08 Sep 2023 16:57


Tgt Ion:202 Resp: 3093
Ion Ratio Lower Upper
202 100
101 153.6 11.4 17.2#
100 1138.2 9.4 14.2#

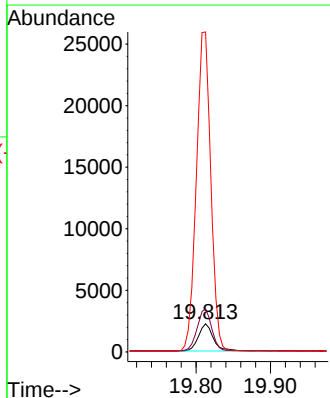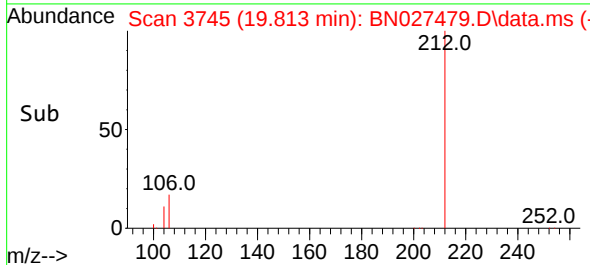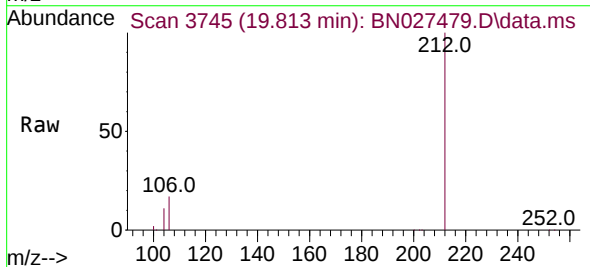

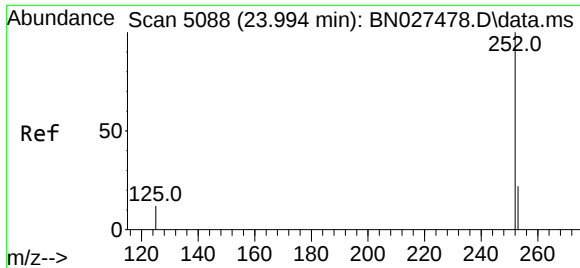

#26
 Benzo(a)pyrene
 Concen: 0.076 ng/ul
 RT: 23.942 min Scan# 50
 Delta R.T. -0.053 min
 Lab File: BN027479.D
 Acq: 08 Sep 2023 16:57

Instrument :
 BNA_N
 ClientSampleId :

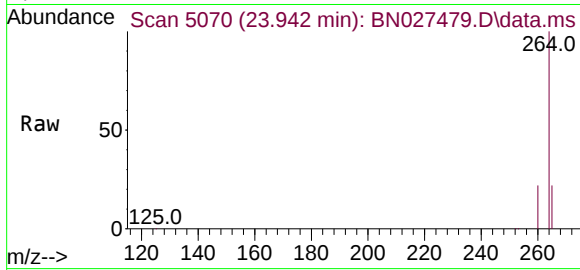

Tgt Ion:252 Resp: 6502

Ion	Ratio	Lower	Upper
252	100		
253	46.6	22.4	33.6#
125	41.3	17.4	26.2#

