

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090823\
 Data File : BN027481.D
 Acq On : 08 Sep 2023 18:13
 Operator : MA/JU
 Sample : PB155241BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 09 00:27:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.046	152	6825	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	23203	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.675	164	14751	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.426	188	33073	0.400	ng/ul	0.00
17) Chrysene-d12	21.598	240	25561	0.400	ng/ul	0.00
23) Perylene-d12	24.106	264	25577	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	59105	6.510	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.445	152	14175	0.403	ng/ul	0.00
18) Fluoranthene-d10	19.446	212	37034	0.423	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.813	202	5312	0.044	ng/ul#	1
26) Benzo(a)pyrene	23.948	252	10356	0.110	ng/ul#	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090823\
Data File : BN027481.D
Acq On : 08 Sep 2023 18:13
Operator : MA/JU
Sample : PB155241BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Sep 09 00:27:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




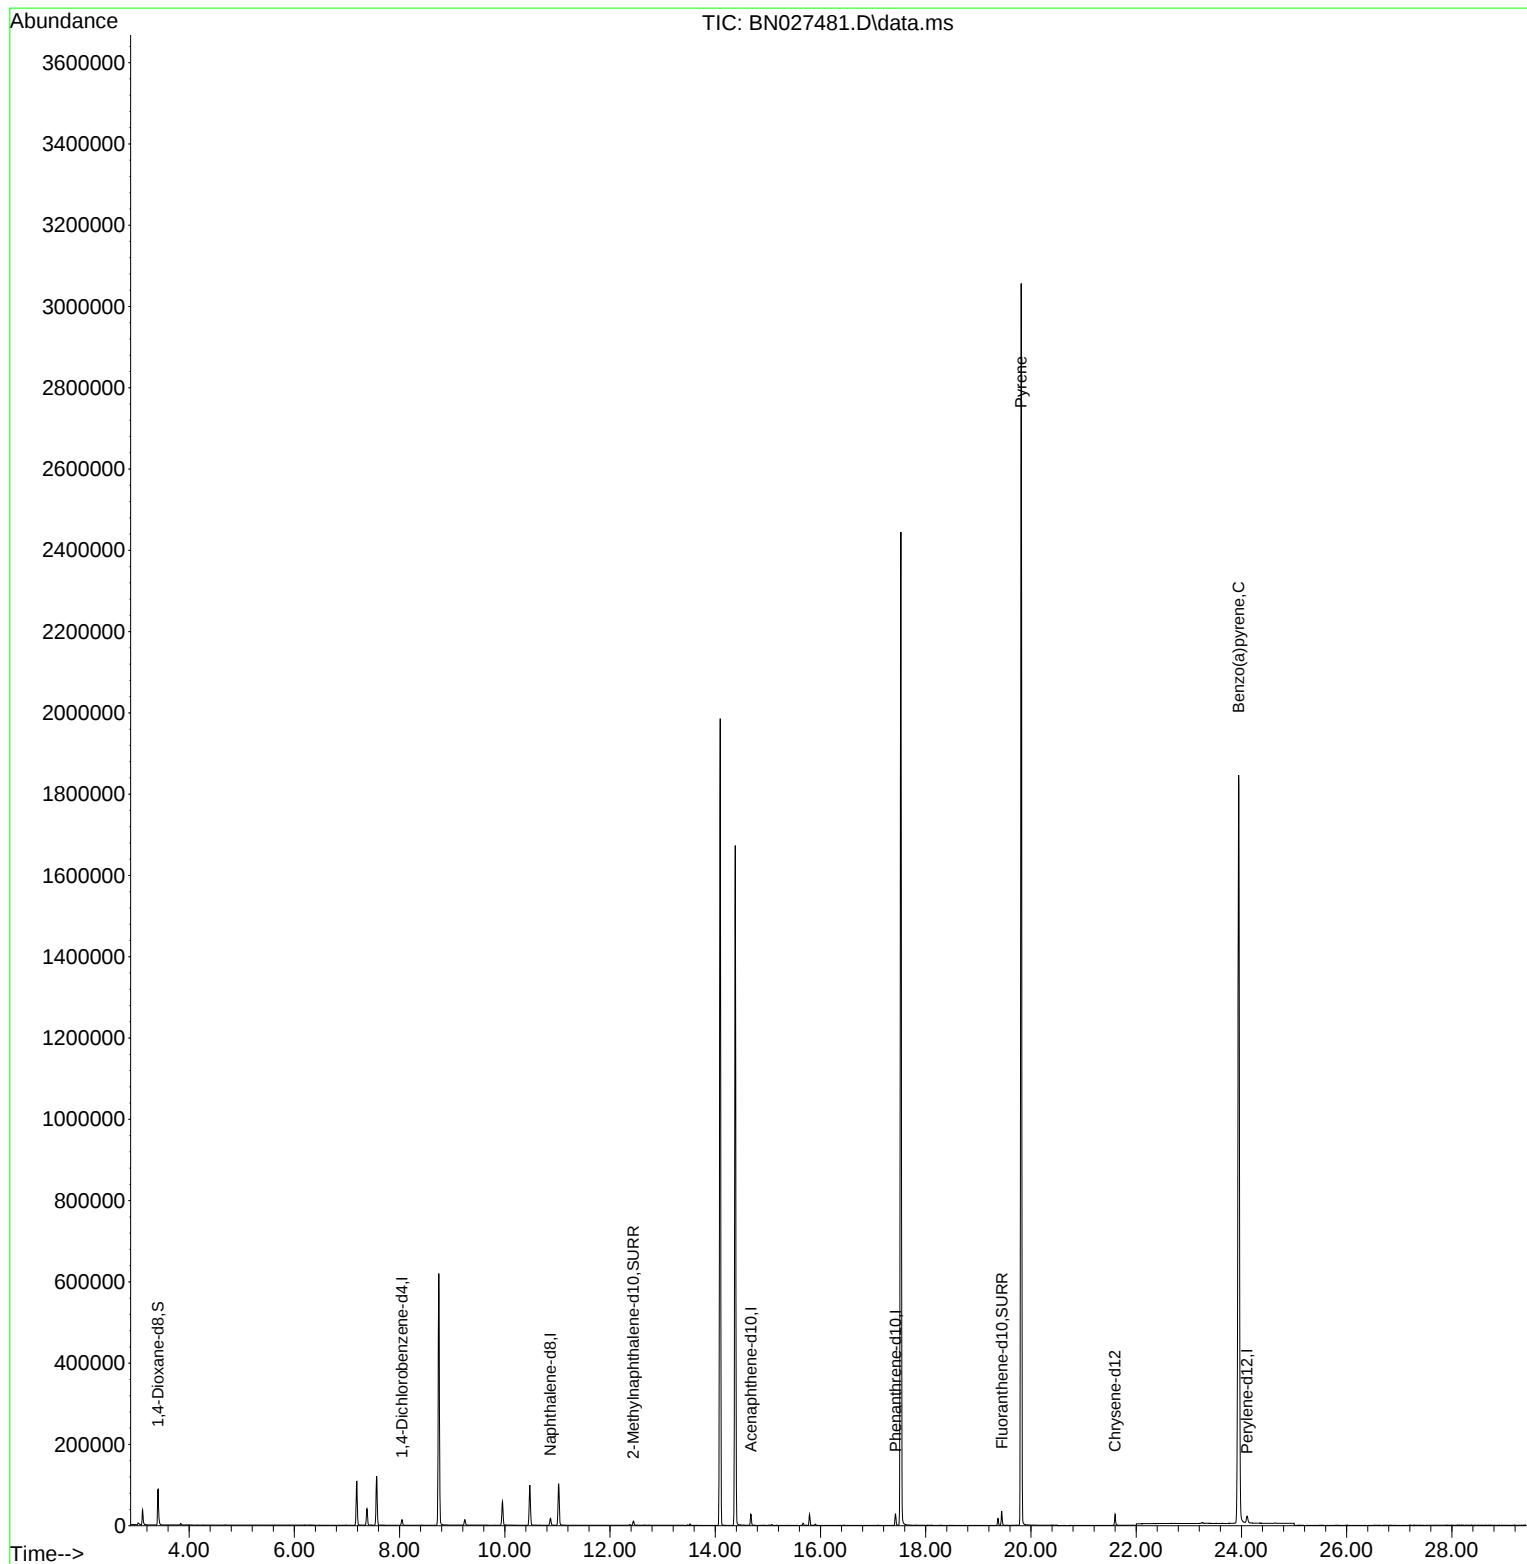


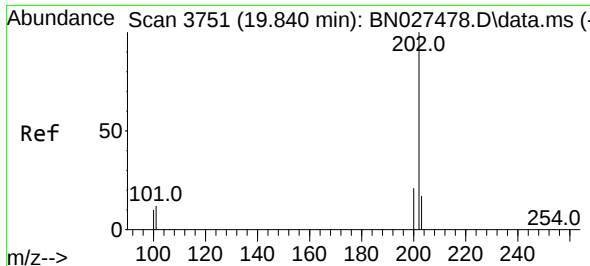

#20
Pyrene
Concen: 0.044 ng/ul
RT: 19.813 min Scan# 31
Delta R.T. -0.028 min
Lab File: BN027481.D
Acq: 08 Sep 2023 18:13

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 5312
Ion Ratio Lower Upper
202 100
101 158.1 11.4 17.2#
100 1190.7 9.4 14.2#

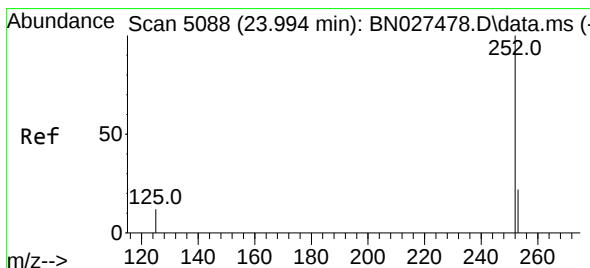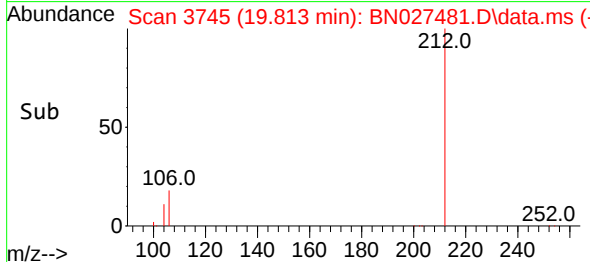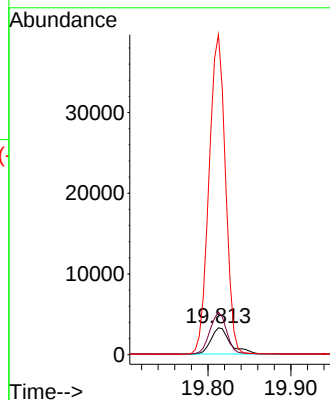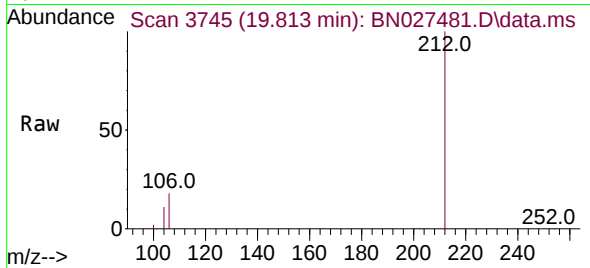

#26
Benzo(a)pyrene
Concen: 0.110 ng/ul
RT: 23.948 min Scan# 5072
Delta R.T. -0.047 min
Lab File: BN027481.D
Acq: 08 Sep 2023 18:13

Tgt Ion:252 Resp: 10356
Ion Ratio Lower Upper
252 100
253 40.7 22.4 33.6#
125 34.1 17.4 26.2#

