

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
 Data File : BN016252.D
 Acq On : 09 Sep 2021 11:01
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Sep 09 14:36:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 09 14:04:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	12843	0.400	ng	0.00
7) Naphthalene-d8	10.660	136	57787	0.400	ng	0.00
13) Acenaphthene-d10	14.497	164	33095	0.400	ng	0.00
19) Phenanthrene-d10	17.237	188	66848	0.400	ng	0.00
29) Chrysene-d12	21.429	240	67446	0.400	ng	# 0.00
35) Perylene-d12	23.823	264	49844	0.400	ng	0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.448	112	154091	4.250	ng	0.00
5) Phenol-d6	7.034	99	199873	4.313	ng	0.00
8) Nitrobenzene-d5	9.013	82	230020	4.958	ng	0.00
11) 2-Methylnaphthalene-d10	12.247	152	441879	4.802	ng	0.00
14) 2,4,6-Tribromophenol	15.982	330	80608	5.458	ng	0.00
15) 2-Fluorobiphenyl	13.114	172	609868	4.888	ng	0.00
27) Fluoranthene-d10	19.276	212	989144	4.928	ng	0.00
31) Terphenyl-d14	19.872	244	828266	4.860	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.364	88	20691	5.036	ng	98
3) n-Nitrosodimethylamine	3.714	42	51648	5.170	ng	# 100
6) bis(2-Chloroethyl)ether	7.292	93	157582	4.701	ng	98
9) Naphthalene	10.711	128	738883	4.831	ng	100
10) Hexachlorobutadiene	10.990	225	148970	4.785	ng	# 100
12) 2-Methylnaphthalene	12.318	142	494418	4.792	ng	99
16) Acenaphthylene	14.218	152	754439	5.081	ng	100
17) Acenaphthene	14.548	154	480102	5.106	ng	97
18) Fluorene	15.537	166	591259	5.006	ng	100
20) 4,6-Dinitro-2-methylph...	15.626	198	50870	10.729	ng	# 51
21) 4-Bromophenyl-phenylether	16.433	248	182955	5.181	ng	97
22) Hexachlorobenzene	16.555	284	205911	4.941	ng	100
23) Atrazine	16.701	200	187109	5.234	ng	98
24) Pentachlorophenol	16.896	266	81427	7.613	ng	98
25) Phenanthrene	17.285	178	946476	5.057	ng	100
26) Anthracene	17.370	178	916706	5.138	ng	100
28) Fluoranthene	19.306	202	1087992	4.902	ng	100
30) Pyrene	19.669	202	1137667	5.178	ng	100
32) Benzo(a)anthracene	21.419	228	1134515	5.009	ng	99
33) Chrysene	21.472	228	1079858	4.906	ng	99
34) Bis(2-ethylhexyl)phtha...	21.344	149	714312	4.684	ng	99
36) Indeno(1,2,3-cd)pyrene	26.298	276	520452	3.754	ng	100
37) Benzo(b)fluoranthene	23.098	252	973319	5.719	ng	98
38) Benzo(k)fluoranthene	23.146	252	875719	5.619	ng	98
39) Benzo(a)pyrene	23.717	252	778902	5.156	ng	96
40) Dibenzo(a,h)anthracene	26.319	278	432163	3.735	ng	94
41) Benzo(g,h,i)perylene	27.058	276	409623	3.517	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016252.D
Acq On : 09 Sep 2021 11:01
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Quant Time: Sep 09 14:36:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 09 14:04:29 2021
Response via : Initial Calibration









1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.864 min Scan# 519
 Delta R.T. -0.000 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	152	Resp:	12843
Ion	Ratio	Lower	Upper
152	100		
150	158.0	125.6	188.4
115	60.0	50.2	75.2



1,4-Dioxane
 Concen: 5.036 ng
 RT: 3.364 min Scan# 31
 Delta R.T. -0.009 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01

Tgt Ion:	88	Resp:	20691
Ion	Ratio	Lower	Upper
88	100		
43	24.0	20.3	30.5
58	86.0	69.9	104.9









#3
 n-Nitrosodimethylamine
 Concen: 5.170 ng
 RT: 3.714 min Scan# 69
 Delta R.T. -0.028 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	42	Resp:	51648
Ion	Ratio	Lower	Upper
42	100		
74	142.3	113.6	170.4
44	8.5	0.0	0.0#



#4
 2-Fluorophenol
 Concen: 4.250 ng
 RT: 5.448 min Scan# 257
 Delta R.T. -0.009 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01

Tgt Ion:	112	Resp:	154091
Ion	Ratio	Lower	Upper
112	100		
64	58.1	47.3	70.9
63	28.1	23.4	35.0









Phenol-d6
 Concen: 4.313 ng
 RT: 7.034 min Scan# 429
 Delta R.T. -0.000 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	99	Resp:	199873
Ion	Ratio	Lower	Upper
99	100		
42	17.1	14.0	21.0
71	29.8	23.8	35.6



bis(2-Chloroethyl)ether
 Concen: 4.701 ng
 RT: 7.292 min Scan# 457
 Delta R.T. -0.000 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01

Tgt Ion:	93	Resp:	157582
Ion	Ratio	Lower	Upper
93	100		
63	76.8	63.4	95.0
95	32.5	26.8	40.2









Naphthalene-d8
 Concen: 0.400 ng
 RT: 10.660 min Scan# 753
 Delta R.T. -0.000 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:	136	Resp:	57787
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.8	13.2
54	5.7	5.3	7.9
68	4.3	3.9	5.9



Nitrobenzene-d5
 Concen: 4.958 ng
 RT: 9.013 min Scan# 623
 Delta R.T. -0.000 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01

Tgt Ion:	82	Resp:	230020
Ion	Ratio	Lower	Upper
82	100		
128	45.2	31.7	47.5
54	52.0	46.4	69.6









Naphthalene
Concen: 4.831 ng
RT: 10.711 min Scan# 757
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt	Ion:128	Resp:	738883
Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.9	13.3
127	12.4	10.1	15.1




Hexachlorobutadiene
Concen: 4.785 ng
RT: 10.990 min Scan# 779
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion:225	Resp: 148970		
Ion Ratio	Lower	Upper	
225 100			
223 0.0	0.0	0.0	
227 64.2	51.5	77.3	






Abundance Scan 986 (12.247 min): BN016256.D\data.ms (-975) (-)




2-Methylnaphthalene-d10
Concen: 4.802 ng
RT: 12.247 min Scan# 986
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:152 Resp: 441879
Ion Ratio Lower Upper
152 100
151 20.0 16.1 24.1






Abundance Scan 1002 (12.318 min): BN016256.D\data.ms (-992) (-)



2-Methylnaphthalene
Concen: 4.792 ng
RT: 12.318 min Scan# 1002
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Tgt Ion:142 Resp: 494418
Ion Ratio Lower Upper
142 100
141 86.9 69.8 104.8
115 30.0 24.4 36.6





Abundance Scan 1201 (14.497 min): BN016256.D\data.ms (-1196) (-)

Acenaphthene-d10
Concen: 0.400 ng
RT: 14.497 min Scan# 1201
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	164	Resp:	33095
Ion Ratio	Lower	Upper	
164	100		
162	97.1	79.0	118.4
160	41.2	34.1	51.1





Abundance Scan 1201 (14.497 min): BN016252.D\data.ms (-1185) (-)




Abundance Scan 1318 (15.982 min): BN016256.D\data.ms (-1314) (-)

2,4,6-Tribromophenol
Concen: 5.458 ng
RT: 15.982 min Scan# 1318
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Tgt Ion:	330	Resp:	80608
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	30.9	25.0	37.4



Abundance Scan 1318 (15.982 min): BN016252.D\data.ms (-1310) (-)





Abundance Scan 1092 (13.114 min): BN016256.D\data.ms (-1084) (-)




2-Fluorobiphenyl
Concen: 4.888 ng
RT: 13.114 min Scan# 1092
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	172	Resp:	609868
Ion	Ratio	Lower	Upper
172	100		
171	34.7	27.8	41.6
170	22.5	18.2	27.2



Abundance Scan 1092 (13.114 min): BN016252.D\data.ms (-1084) (-)





Abundance Scan 1178 (14.205 min): BN016256.D\data.ms (-1118) (-)




Acenaphthylene
Concen: 5.081 ng
RT: 14.218 min Scan# 1179
Delta R.T. 0.013 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion:	152	Resp:	754439
Ion	Ratio	Lower	Upper
152	100		
151	19.0	15.2	22.8
153	13.1	10.5	15.7




Abundance Scan 1179 (14.218 min): BN016252.D\data.ms (-1162) (-)





Abundance Scan 1205 (14.548 min): BN016256.D\data.ms (-1205) (-)

Acenaphthene
Concen: 5.106 ng
RT: 14.548 min Scan# 1205
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Instrument :
BNA_N
ClientSampled :
SSTDICC5.0



Tgt Ion:	154	Resp:	480102
Ion	Ratio	Lower	Upper
154	100		
153	108.3	89.3	133.9
152	49.9	42.2	63.4




Abundance Scan 1205 (14.548 min): BN016252.D\data.ms (-1197) (-)





Abundance Scan 1283 (15.538 min): BN016256.D\data.ms (-1218) (-)


Fluorene
Concen: 5.006 ng
RT: 15.537 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01



Tgt Ion:	166	Resp:	591259
Ion	Ratio	Lower	Upper
166	100		
165	95.7	76.7	115.1
167	13.6	10.9	16.3




Abundance Scan 1283 (15.537 min): BN016252.D\data.ms (-1267) (-)





Abundance Scan 1421 (17.237 min): BN016256.D\data.ms (-1419) (-)

Phenanthrene-d10
Concen: 0.400 ng
RT: 17.237 min Scan# 1421
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion:	188	Resp:	66848
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	9.5	7.0	10.6





Abundance Scan 1421 (17.237 min): BN016252.D\data.ms (-1405) (-)




Abundance Scan 1291 (15.639 min): BN016256.D\data.ms (-1286) (-)

4,6-Dinitro-2-methylphenol
Concen: 10.729 ng
RT: 15.626 min Scan# 1290
Delta R.T. -0.013 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Tgt Ion:	198	Resp:	50870
Ion Ratio	Lower	Upper	
198	100		
182	5.6	26.6	39.8#
77	0.0	0.0	0.0



Abundance Scan 1290 (15.626 min): BN016252.D\data.ms (-1283) (-)





Abundance Scan 1355 (16.433 min): BN016256.D\data.ms (-1320) (-)




4-Bromophenyl-phenylether
Concen: 5.181 ng
RT: 16.433 min Scan# 1355
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion	Ratio	Lower	Upper
248	100		
250	102.5	80.5	120.7
141	40.8	34.8	52.2



Abundance Scan 1355 (16.433 min): BN016252.D\data.ms (-1347) (-)





Abundance Scan 1365 (16.555 min): BN016256.D\data.ms (-1329) (-)




Hexachlorobenzene
Concen: 4.941 ng
RT: 16.555 min Scan# 1365
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion	Ratio	Lower	Upper
284	100		
142	28.3	22.6	34.0
249	30.8	24.4	36.6




Abundance Scan 1365 (16.555 min): BN016252.D\data.ms (-1357) (-)





Abundance Scan 1377 (16.701 min): BN016256.D\data.ms (-1329) (-)

Atrazine
Concen: 5.234 ng
RT: 16.701 min Scan# 1377
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0



Tgt Ion	Ratio	Lower	Upper
200	100		
173	24.1	18.7	28.1
215	50.7	41.6	62.4






Abundance Scan 1377 (16.701 min): BN016252.D\data.ms (-1336) (-)




Abundance Scan 1393 (16.896 min): BN016256.D\data.ms (-1327) (-)

Pentachlorophenol
Concen: 7.613 ng
RT: 16.896 min Scan# 1393
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Tgt Ion	Ratio	Lower	Upper
266	100		
264	62.6	50.6	75.8
268	63.8	52.6	79.0



Abundance Scan 1393 (16.896 min): BN016252.D\data.ms (-1385) (-)






Abundance Scan 1424 (17.273 min): BN016256.D\data.ms (-1424) (-)




Phenanthrene
Concen: 5.057 ng
RT: 17.285 min Scan# 1425
Delta R.T. 0.012 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	178	Resp:	946476
Ion	Ratio	Lower	Upper
178	100		
176	17.9	14.4	21.6
179	15.4	12.2	18.4






Abundance Scan 1432 (17.371 min): BN016256.D\data.ms (-1426) (-)




Anthracene
Concen: 5.138 ng
RT: 17.370 min Scan# 1432
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion:	178	Resp:	916706
Ion	Ratio	Lower	Upper
178	100		
176	17.3	13.9	20.9
179	15.5	12.2	18.4






Abundance Scan 1738 (19.271 min): BN016256.D\data.ms (-1728) (-)




Fluoranthene-d10
Concen: 4.928 ng
RT: 19.276 min Scan# 1739
Delta R.T. 0.005 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:212 Resp: 989144
Ion Ratio Lower Upper
212 100
106 12.2 9.8 14.6
104 6.8 5.4 8.2






Abundance Scan 1744 (19.301 min): BN016256.D\data.ms (-1728) (-)




Fluoranthene
Concen: 4.902 ng
RT: 19.306 min Scan# 1745
Delta R.T. 0.005 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion:202 Resp: 1087992
Ion Ratio Lower Upper
202 100
101 10.6 8.5 12.7
203 17.5 13.8 20.8






Abundance Scan 2020 (21.429 min): BN016256.D\data.ms (-2020) (-)




Chrysene-d12
Concen: 0.400 ng
RT: 21.429 min Scan# 2020
Delta R.T. -0.000 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:	240	Resp:	67446
Ion	Ratio	Lower	Upper
240	100		
120	13.5	5.3	7.9#
236	26.2	19.8	29.8






Abundance Scan 1817 (19.664 min): BN016256.D\data.ms (-1817) (-)



Pyrene
Concen: 5.178 ng
RT: 19.669 min Scan# 1818
Delta R.T. 0.005 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01


Tgt Ion:	202	Resp:	1137667
Ion	Ratio	Lower	Upper
202	100		
200	19.7	15.8	23.6
203	17.6	13.9	20.9






Abundance Scan 1858 (19.867 min): BN016256.D\data.ms (-1828) (-)

Terphenyl-d14
Concen: 4.860 ng
RT: 19.872 min Scan# 1859
Delta R.T. 0.005 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

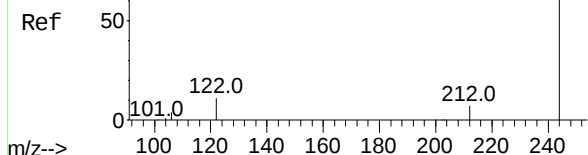


Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.7	5.5	8.3
122	10.4	9.0	13.4







Abundance Scan 2018 (21.408 min): BN016256.D\data.ms (-2009) (-)

Benzo(a)anthracene
Concen: 5.009 ng
RT: 21.419 min Scan# 2019
Delta R.T. 0.011 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01




Tgt Ion	Ratio	Lower	Upper
228	100		
226	25.2	20.8	31.2
229	20.0	15.8	23.6








Chrysene
 Concen: 4.906 ng
 RT: 21.472 min Scan# 2024
 Delta R.T. 0.011 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01


Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0





Tgt Ion:	228	Resp:	1079858
Ion	Ratio	Lower	Upper
228	100		
226	28.1	23.0	34.4
229	20.0	15.6	23.4



Bis(2-ethylhexyl)phthalate
 Concen: 4.684 ng
 RT: 21.344 min Scan# 2012
 Delta R.T. 0.011 min
 Lab File: BN016252.D
 Acq: 09 Sep 2021 11:01




Tgt Ion:	149	Resp:	714312
Ion	Ratio	Lower	Upper
149	100		
167	29.6	23.4	35.0
279	4.9	3.9	5.9






Abundance Scan 2523 (23.813 min): BN016256.D\data.ms (-2535) (-)

Perylene-d12
Concen: 0.400 ng
RT: 23.823 min Scan# 2526
Delta R.T. 0.010 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampled :
SSTDICC5.0




Tgt Ion:	264	Resp:	49844
Ion Ratio	Lower	Upper	
264	100		
260	23.6	18.9	28.3
265	26.9	23.7	35.5






Abundance Scan 3246 (26.288 min): BN016256.D\data.ms (-3226) (-)


Indeno(1,2,3-cd)pyrene
Concen: 3.754 ng
RT: 26.298 min Scan# 3249
Delta R.T. 0.010 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01



Tgt Ion:	276	Resp:	520452
Ion Ratio	Lower	Upper	
276	100		
138	23.9	19.3	28.9
277	25.2	20.2	30.2






Abundance Scan 2311 (23.087 min): BN016256.D\data.ms (-2253) (-)




Benzo(b)fluoranthene
Concen: 5.719 ng
RT: 23.098 min Scan# 2314
Delta R.T. 0.010 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion:	252	Resp:	973319
Ion	Ratio	Lower	Upper
252	100		
253	22.1	18.2	27.2
125	9.4	8.4	12.6






Abundance Scan 2325 (23.135 min): BN016256.D\data.ms (-2310) (-)



Benzo(k)fluoranthene
Concen: 5.619 ng
RT: 23.146 min Scan# 2328
Delta R.T. 0.010 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Tgt Ion:	252	Resp:	875719
Ion	Ratio	Lower	Upper
252	100		
253	22.1	18.2	27.2
125	9.3	8.2	12.4




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Abundance Scan 2492 (23.707 min): BN016256.D\data.ms (-2434) (-)

Benzo(a)pyrene
Concen: 5.156 ng
RT: 23.717 min Scan# 2495
Delta R.T. 0.010 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0




Tgt Ion:	252	Resp:	778902
Ion	Ratio	Lower	Upper
252	100		
253	21.9	18.7	28.1
125	10.3	9.9	14.9






Abundance Scan 3252 (26.308 min): BN016256.D\data.ms (-3223) (-)


Dibenzo(a,h)anthracene
Concen: 3.735 ng
RT: 26.319 min Scan# 3255
Delta R.T. 0.010 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01



Tgt Ion:	278	Resp:	432163
Ion	Ratio	Lower	Upper
278	100		
139	14.8	14.2	21.2
279	23.7	21.3	31.9




Abundance Scan 3467 (27.044 min): BN016256.D\data.ms (-3442) (-)



Benzo(g,h,i)perylene
Concen: 3.517 ng
RT: 27.058 min Scan# 3471
Delta R.T. 0.014 min
Lab File: BN016252.D
Acq: 09 Sep 2021 11:01

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Abundance Scan 3471 (27.058 min): BN016252.D\data.ms



Tgt Ion:	276	Resp:	409623
Ion	Ratio	Lower	Upper
276	100		
277	24.0	20.5	30.7
138	20.6	18.2	27.4

Abundance Scan 3471 (27.058 min): BN016252.D\data.ms (-3409) (-)

