
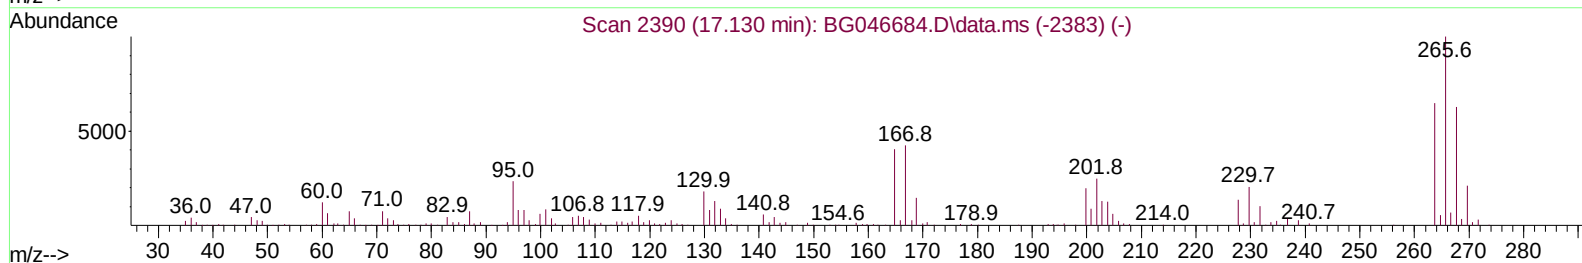
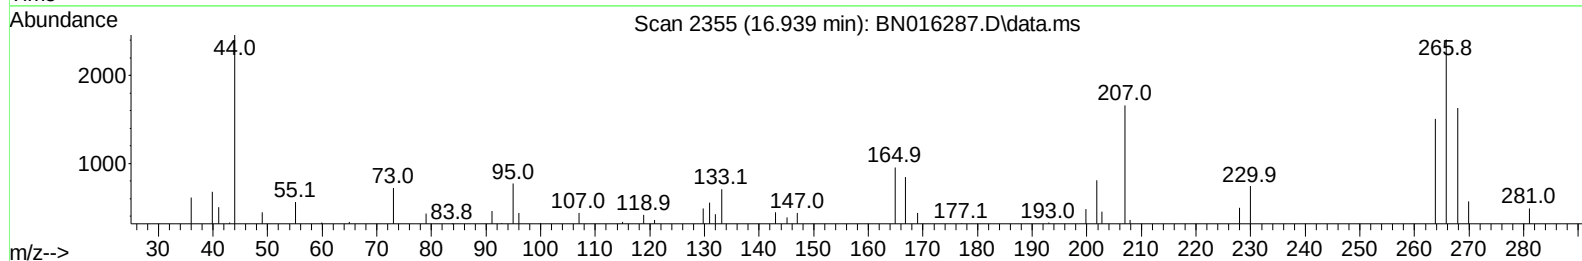


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016287.D
Acq On : 10 Sep 2021 10:34
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Sep 10 13:00:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

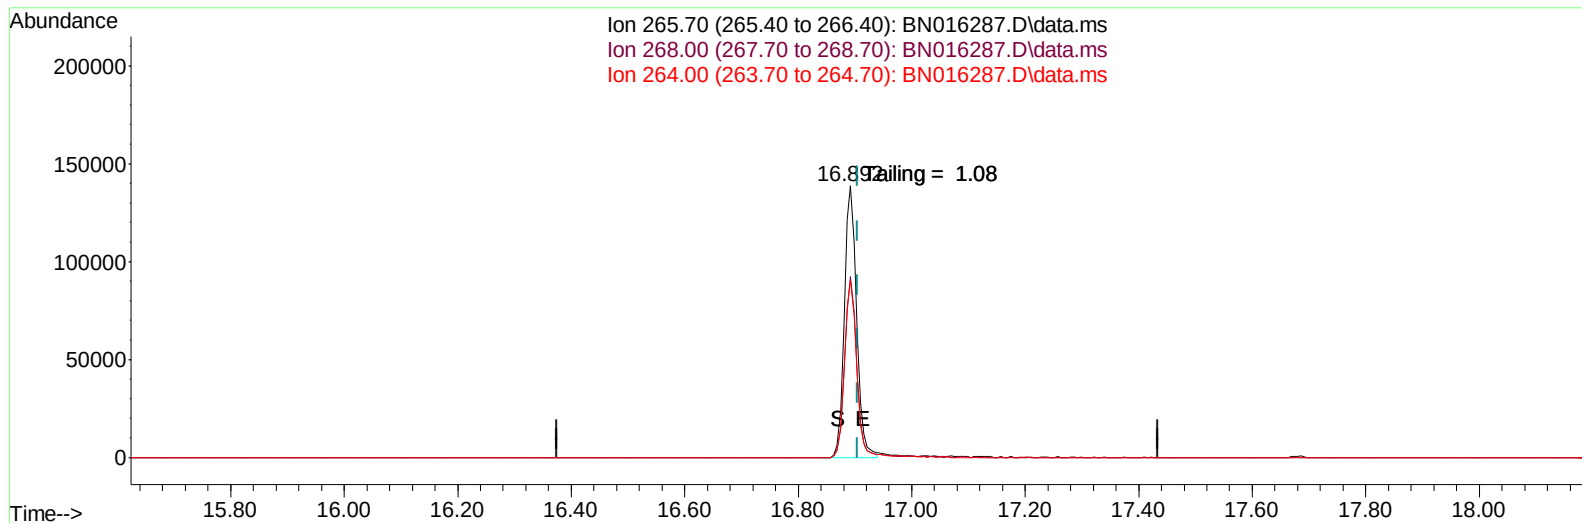

TIC: BN016287.D\data.ms

(70) Pentachlorophenol (C)




16.939min (+ 0.035) 137.17 ng m

response 1379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.73
264.00	61.60	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016287.D
Acq On : 10 Sep 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Quant Time: Sep 10 13:00:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

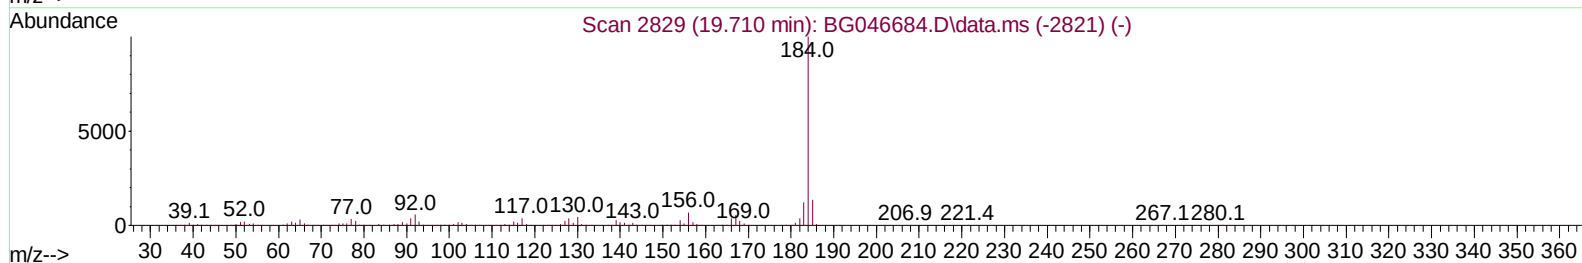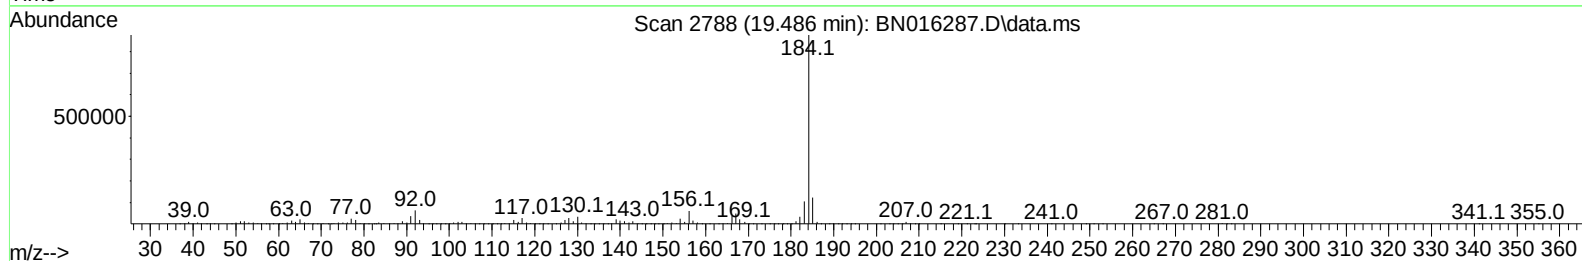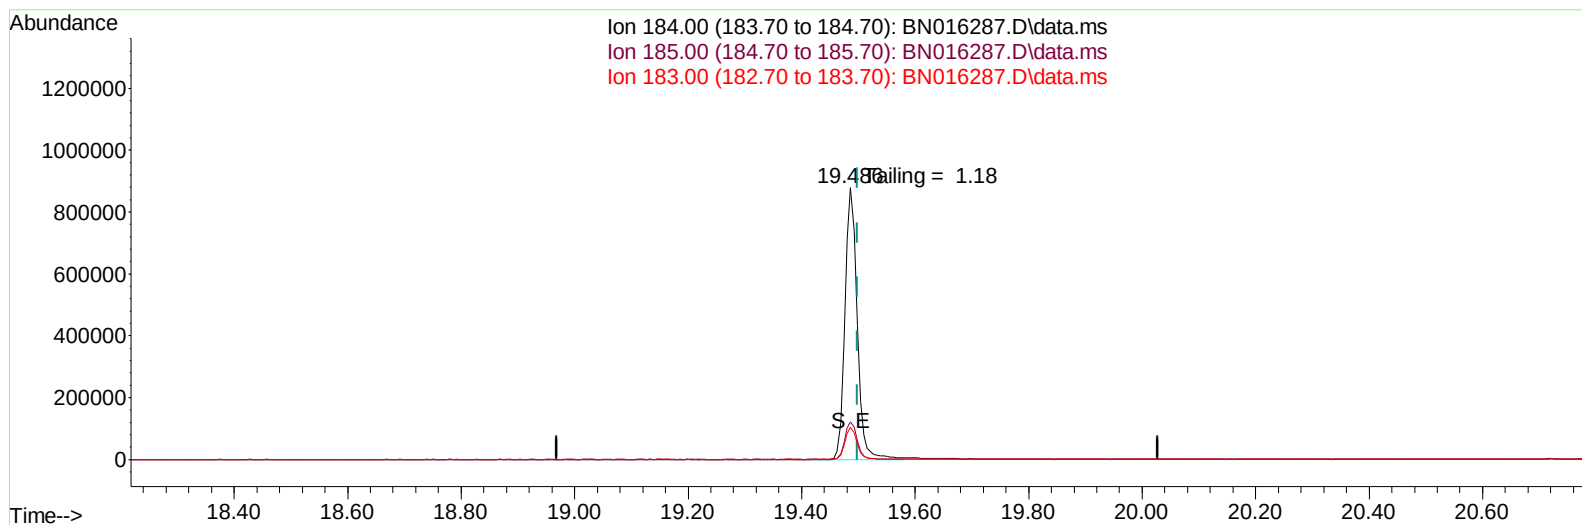

TIC: BN016287.D\data.ms

(77) Benzidine**19.486min (-0.012) 41434.32 ng****response 1320654**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.94
0.00	0.00	0.00