

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
 Data File : BN016279.D
 Acq On : 10 Sep 2021 05:44
 Operator : CG/JU
 Sample : M3620-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BP-TT-VPB-RW7-GW-640-642

Manual Integrations
 APPROVED

mohammad
 9/10/2021 3:24:04 PM

Quant Time: Sep 10 06:12:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 09 15:19:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.864	152	12558	0.400	ng	0.00
7) Naphthalene-d8	10.660	136	64556	0.400	ng	0.00
13) Acenaphthene-d10	14.484	164	36991	0.400	ng	-0.01
19) Phenanthrene-d10	17.237	188	73558	0.400	ng	0.00
29) Chrysene-d12	21.429	240	69928	0.400	ng	0.00
35) Perylene-d12	23.810	264	47932	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.457	112	2456	0.077	ng	0.00
5) Phenol-d6	7.034	99	2027	0.051	ng	0.00
8) Nitrobenzene-d5	9.013	82	13940	0.269	ng	0.00
11) 2-Methylnaphthalene-d10	12.243	152	26670	0.265	ng	0.00
14) 2,4,6-Tribromophenol	15.982	330	2871	0.189	ng	0.00
15) 2-Fluorobiphenyl	13.114	172	38793	0.268	ng	0.00
27) Fluoranthene-d10	19.271	212	74226	0.343	ng	0.00
31) Terphenyl-d14	19.867	244	70770	0.403	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.373	88	9781m	2.195	ng	
9) Naphthalene	10.698	128	9373	0.054	ng	97
12) 2-Methylnaphthalene	12.318	142	9558	0.082	ng	99
17) Acenaphthene	14.548	154	5149	0.048	ng	# 73
18) Fluorene	15.537	166	13336	0.100	ng	# 76
24) Pentachlorophenol	16.896	266	833	0.235	ng	97
25) Phenanthrene	17.273	178	82103	0.384	ng	# 92
28) Fluoranthene	19.296	202	6500	0.026	ng	# 91
30) Pyrene	19.664	202	12784	0.054	ng	# 72
34) Bis(2-ethylhexyl)phtha...	21.334	149	38748	0.289	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016279.D
Acq On : 10 Sep 2021 05:44
Operator : CG/JU
Sample : M3620-03
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642

Manual Integrations
APPROVED

mohammad
9/10/2021 3:24:04 PM


Quant Time: Sep 10 06:12:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 09 15:19:08 2021
Response via : Initial Calibration

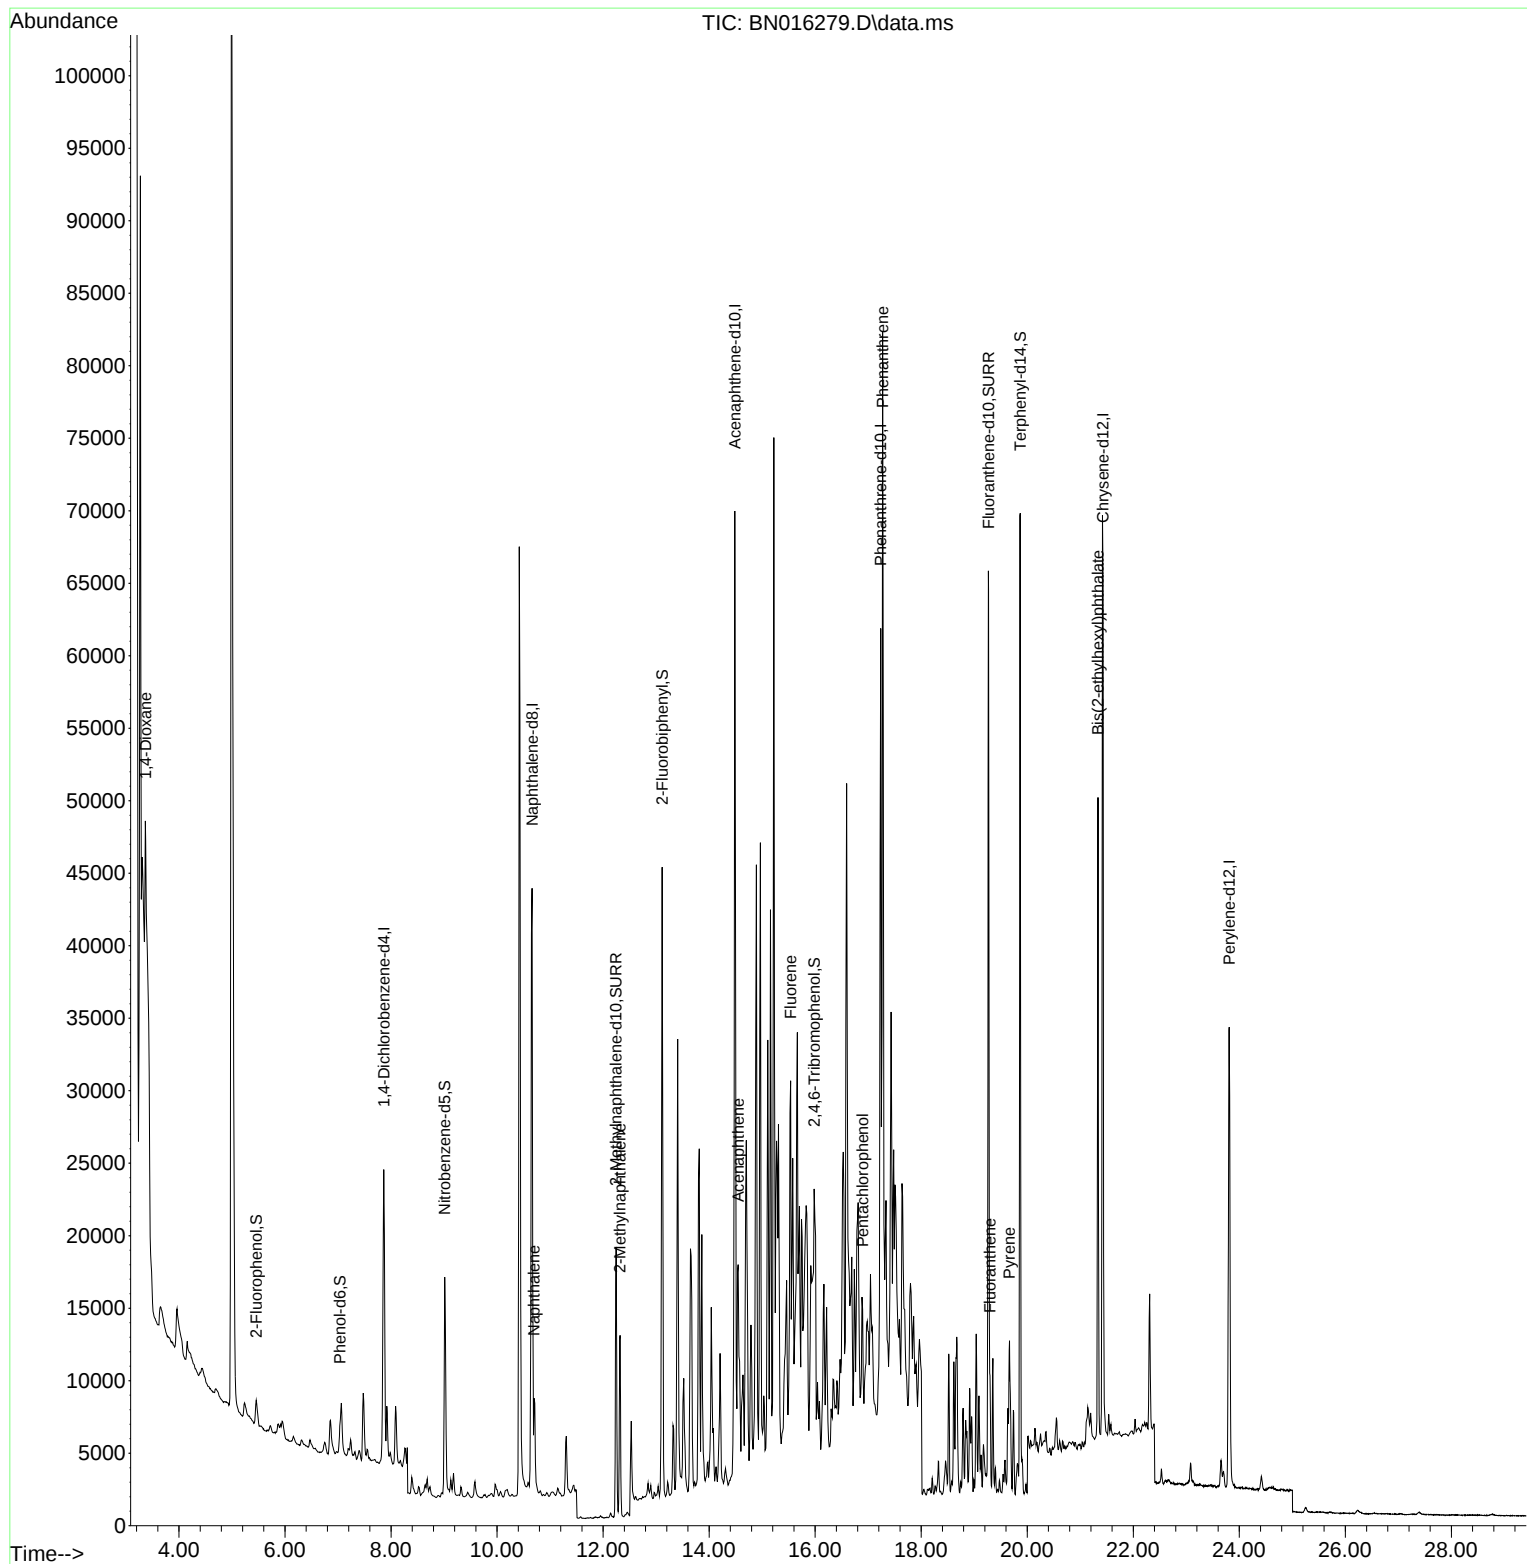

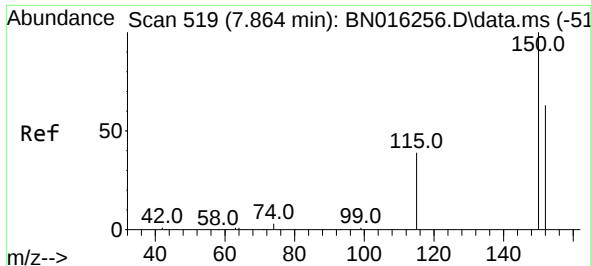

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.864 min Scan# 519
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Tgt Ion:152 Resp: 12558
Ion Ratio Lower Upper
152 100
150 154.5 125.6 188.4
115 60.7 50.2 75.2

Manual Integrations
APPROVED



mohammad
9/10/2021 3:24:04 PM

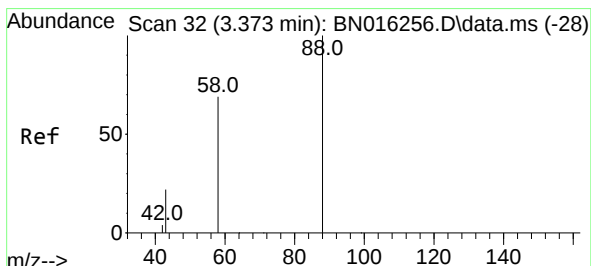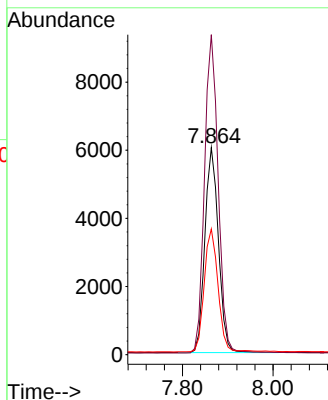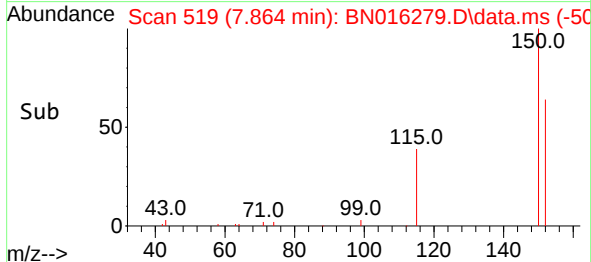


#2
1,4-Dioxane
Concen: 2.195 ng m
RT: 3.373 min Scan# 32
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

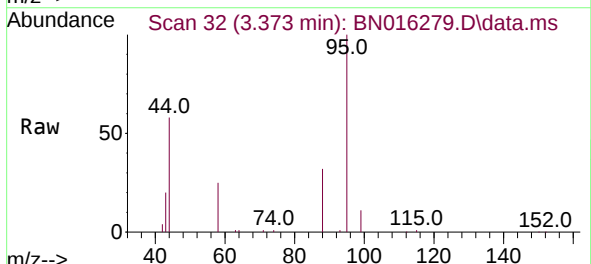

Tgt Ion: 88 Resp: 9781
Ion Ratio Lower Upper
88 100
43 37.6 20.3 30.5#
58 111.2 69.9 104.9#

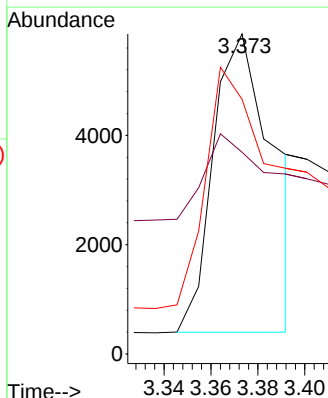

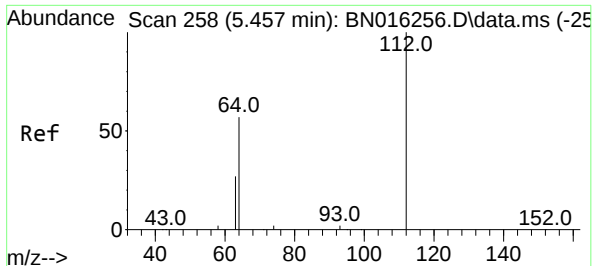





#4
2-Fluorophenol
Concen: 0.077 ng
RT: 5.457 min Scan# 258
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.4	47.3	70.9
63	29.3	23.4	35.0

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

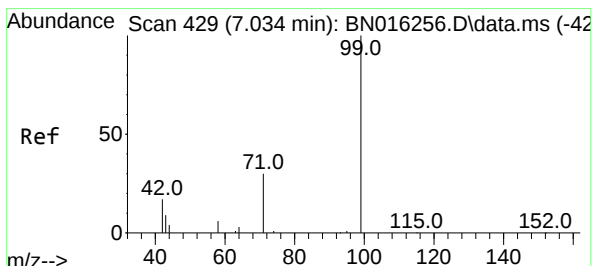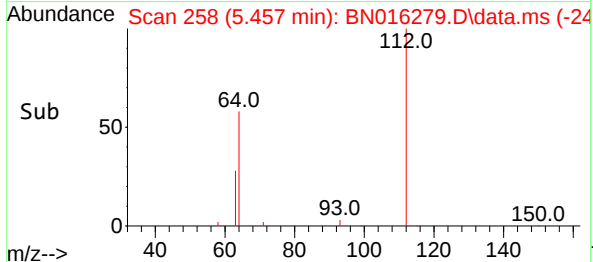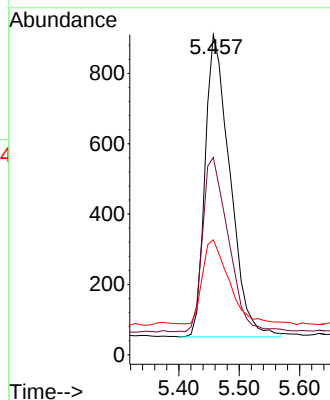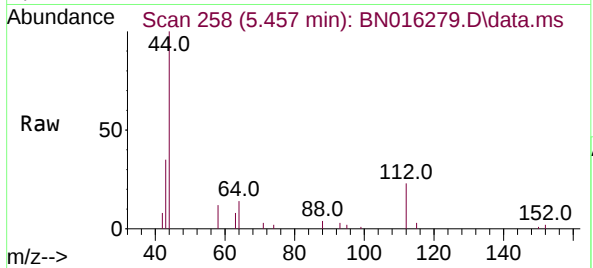

#5
Phenol-d6
Concen: 0.051 ng
RT: 7.034 min Scan# 429
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44


Tgt Ion	Ratio	Lower	Upper
99	100		
42	26.5	14.0	21.0#
71	46.1	23.8	35.6#

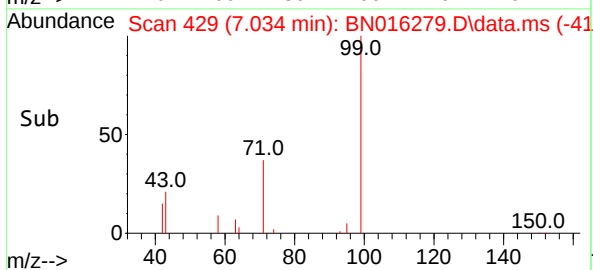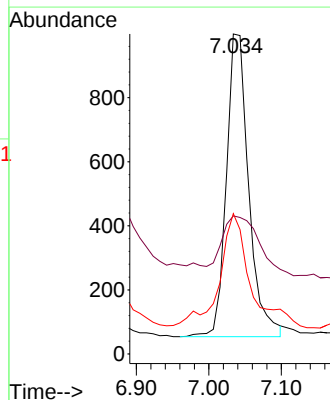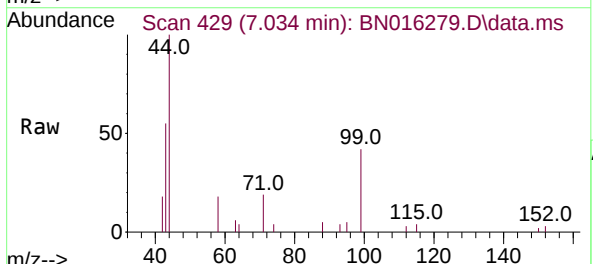

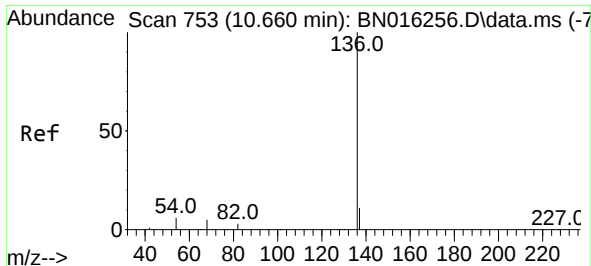

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.660 min Scan# 753
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44



Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Tgt Ion:	136	Resp:	64556
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.8	13.2
54	5.9	5.3	7.9
68	4.4	3.9	5.9

Manual Integrations
APPROVED



mohammad
9/10/2021 3:24:04 PM

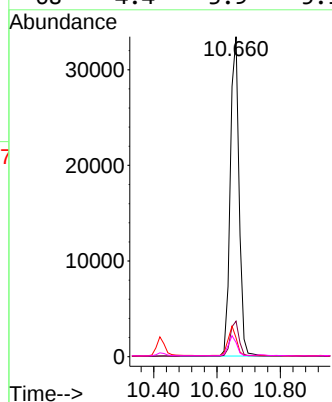


#8
Nitrobenzene-d5
Concen: 0.269 ng
RT: 9.013 min Scan# 623
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

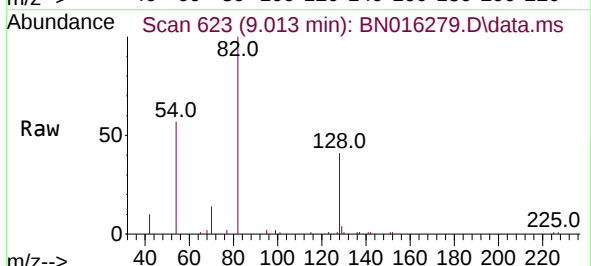

Tgt Ion:	82	Resp:	13940
Ion	Ratio	Lower	Upper
82	100		
128	41.2	31.7	47.5
54	57.1	46.4	69.6

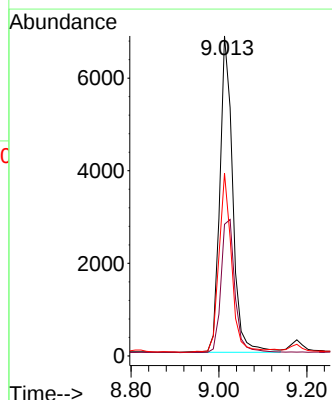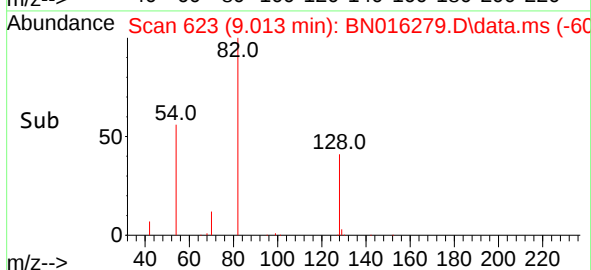

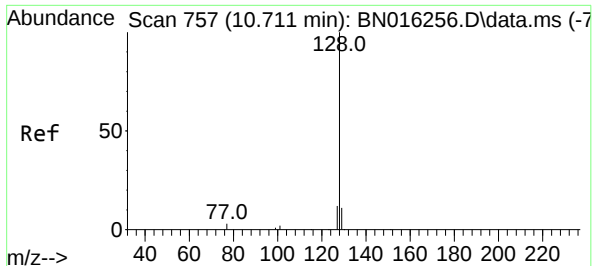





#9
Naphthalene
Concen: 0.054 ng
RT: 10.698 min Scan# 756
Delta R.T. -0.013 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion	Ratio	Lower	Upper
128	100		
129	12.3	8.9	13.3
127	14.1	10.1	15.1

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

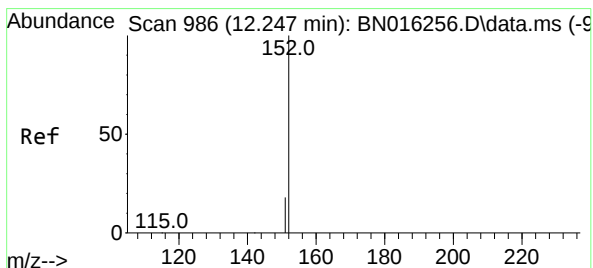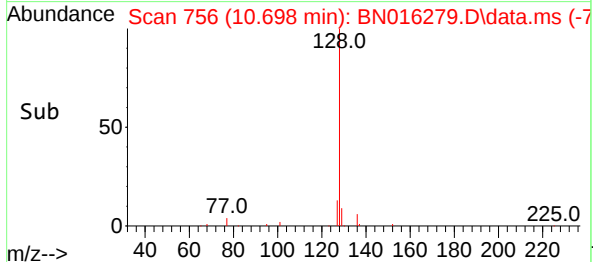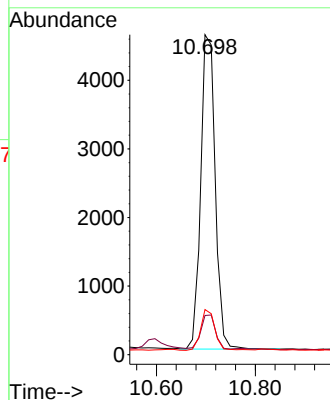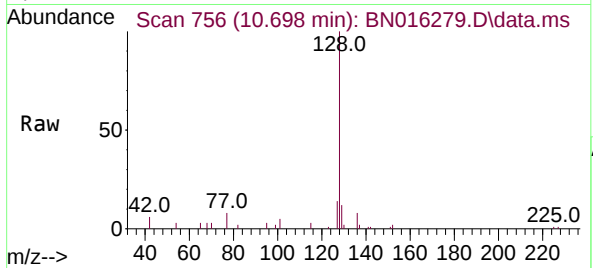

#11
2-Methylnaphthalene-d10
Concen: 0.265 ng
RT: 12.243 min Scan# 985
Delta R.T. -0.005 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44


Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.6	16.1	24.1

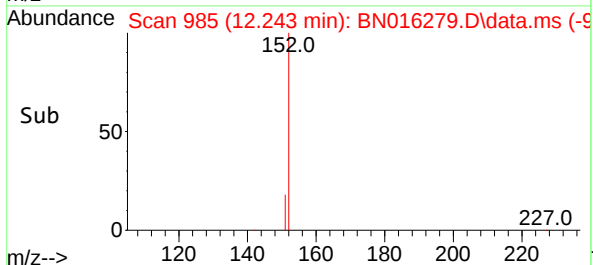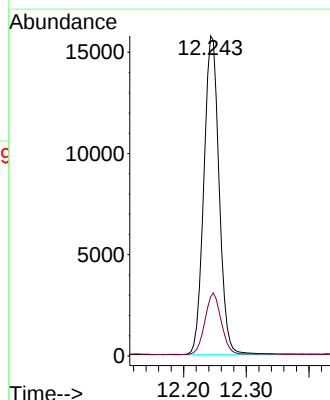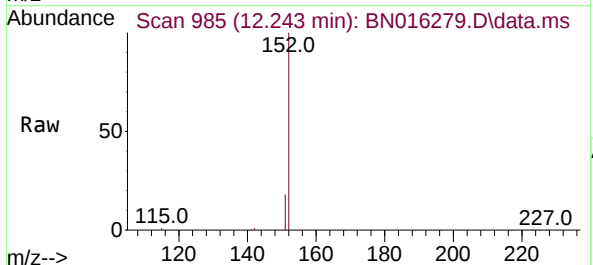

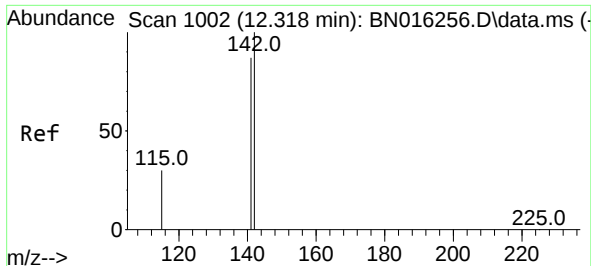

#12
2-Methylnaphthalene
Concen: 0.082 ng
RT: 12.318 min Scan# 1002
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Tgt Ion:142 Resp: 9558
Ion Ratio Lower Upper
142 100
141 87.8 69.8 104.8
115 31.3 24.4 36.6

Manual Integrations
APPROVED



mohammad
9/10/2021 3:24:04 PM

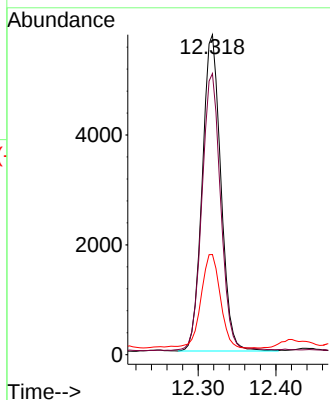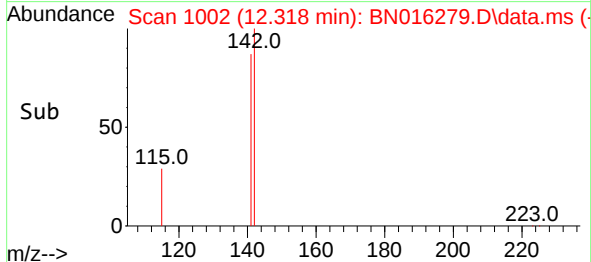


#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.484 min Scan# 1200
Delta R.T. -0.013 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

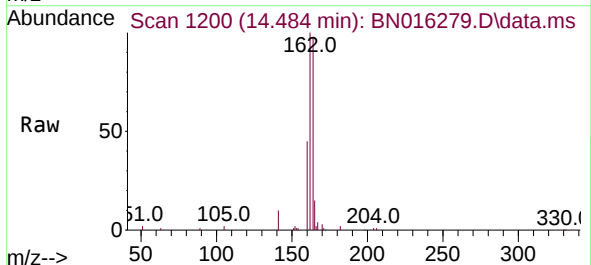

Tgt Ion:164 Resp: 36991
Ion Ratio Lower Upper
164 100
162 102.0 79.0 118.4
160 45.8 34.1 51.1

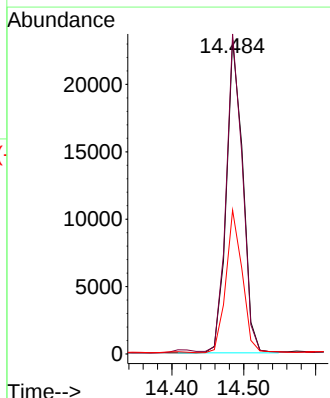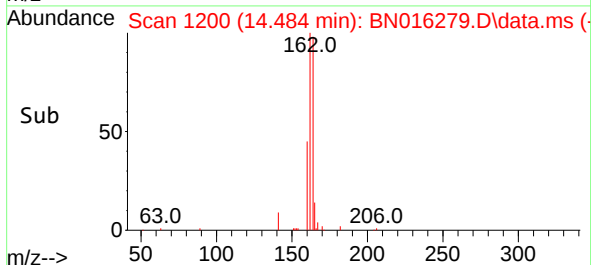

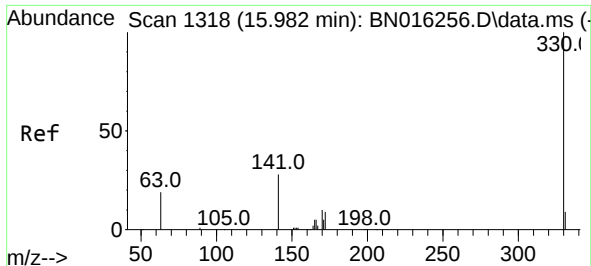





#14
2,4,6-Tribromophenol
Concen: 0.189 ng
RT: 15.982 min Scan# 1318
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion: 330 Resp: 2871
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 85.1 25.0 37.4#

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

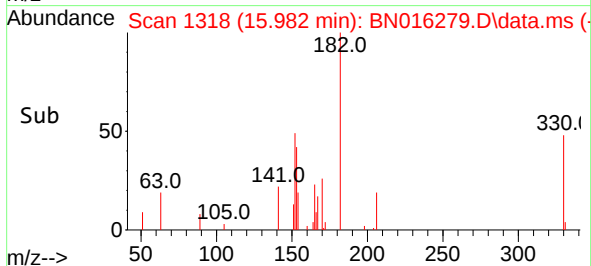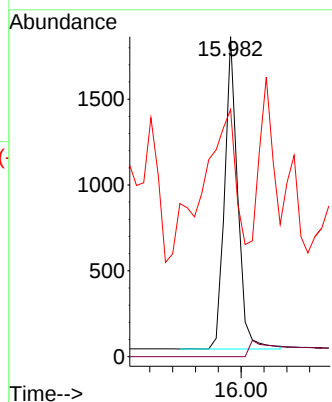

#15
2-Fluorobiphenyl
Concen: 0.268 ng
RT: 13.114 min Scan# 1092
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44


Tgt Ion: 172 Resp: 38793
Ion Ratio Lower Upper
172 100
171 34.5 27.8 41.6
170 22.3 18.2 27.2

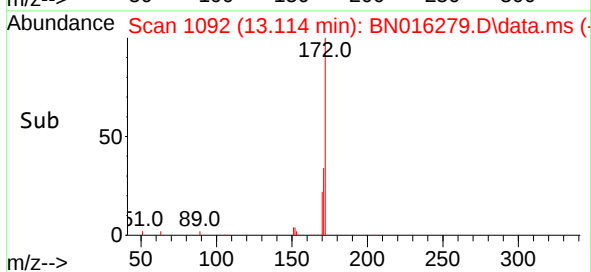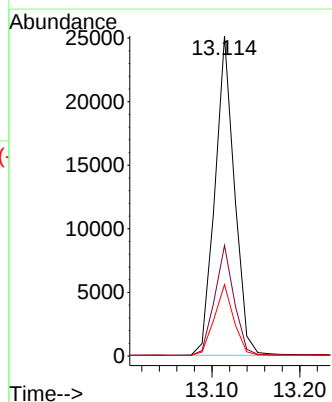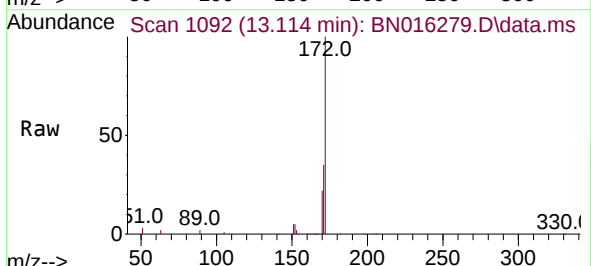



#17
Acenaphthene
Concen: 0.048 ng
RT: 14.548 min Scan# 1205
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44




Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Tgt Ion:154 Resp: 5149
Ion Ratio Lower Upper
154 100
153 134.4 89.3 133.9#
152 79.5 42.2 63.4#

Manual Integrations
APPROVED



mohammad
9/10/2021 3:24:04 PM

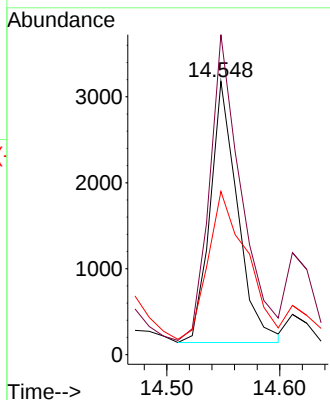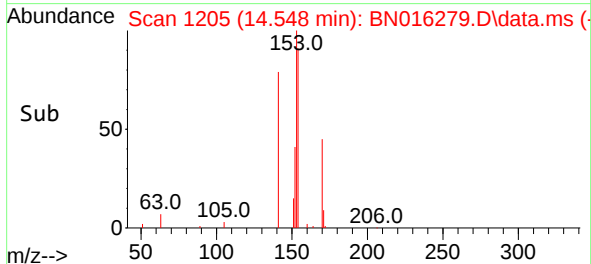


#18
Fluorene
Concen: 0.100 ng
RT: 15.537 min Scan# 1283
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

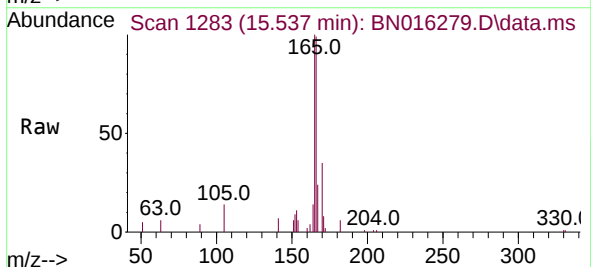

Tgt Ion:166 Resp: 13336
Ion Ratio Lower Upper
166 100
165 118.5 76.7 115.1#
167 25.6 10.9 16.3#

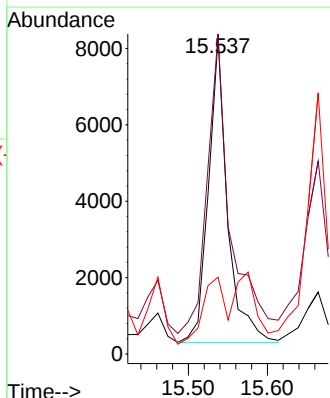

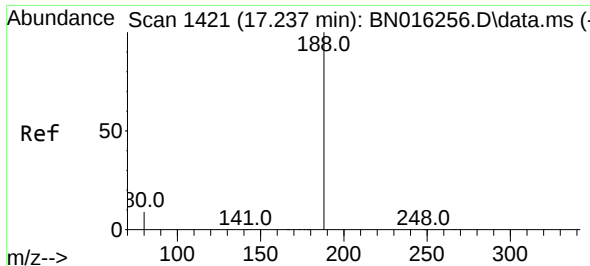





#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.237 min Scan# 1421
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	7.9	7.0	10.6

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

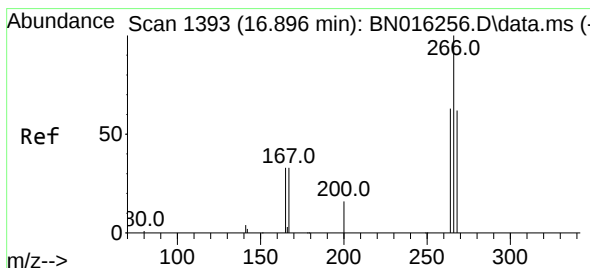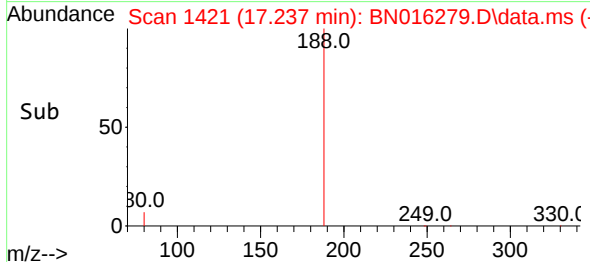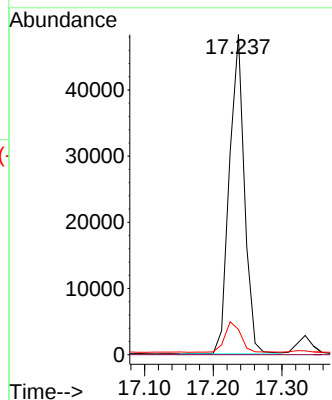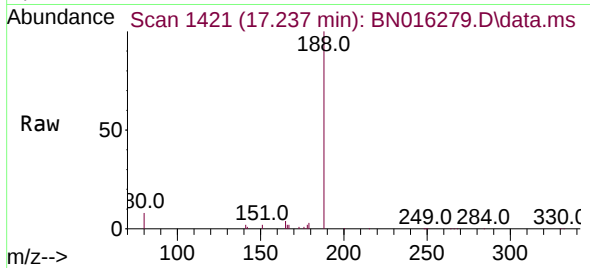

#24
Pentachlorophenol
Concen: 0.235 ng
RT: 16.896 min Scan# 1393
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion	Ratio	Lower	Upper
266	100		
264	65.7	50.6	75.8
268	64.1	52.6	79.0

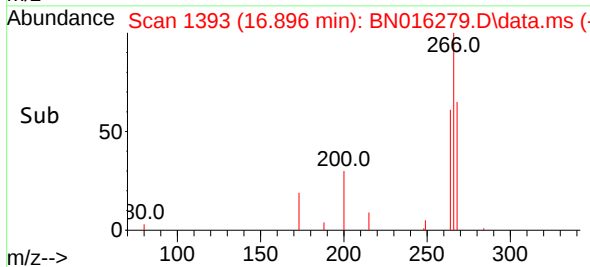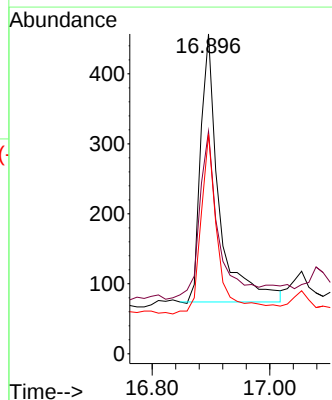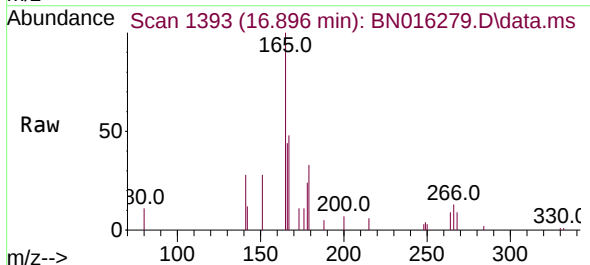

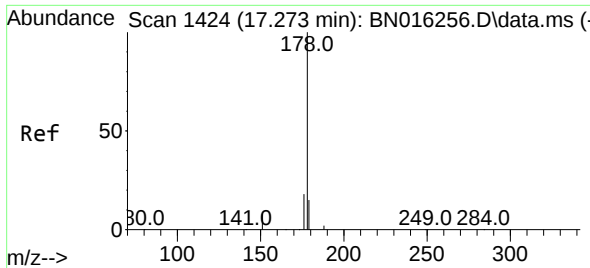





#25
Phenanthrene
Concen: 0.384 ng
RT: 17.273 min Scan# 1424
Delta R.T. 0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion:	178	Resp:	82103
Ion Ratio	Lower	Upper	
178	100		
176	17.2	14.4	21.6
179	21.4	12.2	18.4#

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

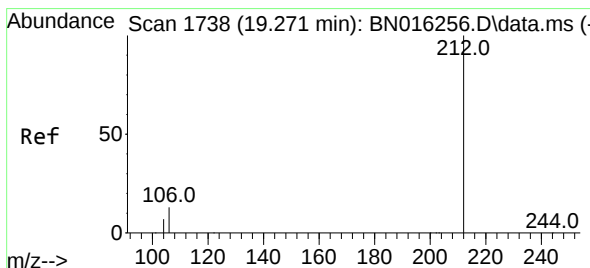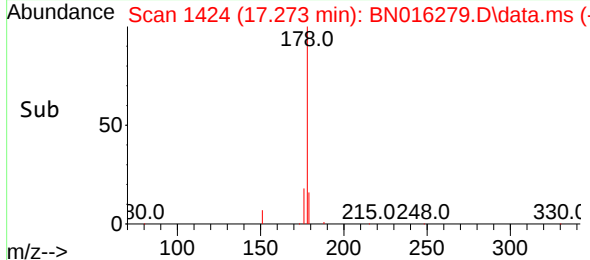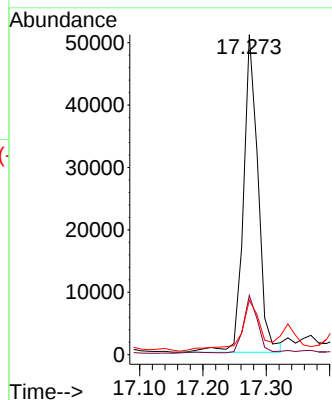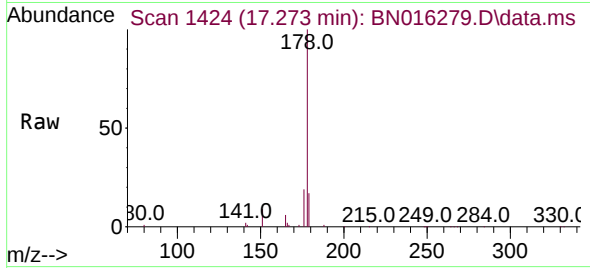

#27
Fluoranthene-d10
Concen: 0.343 ng
RT: 19.271 min Scan# 1738
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion:	212	Resp:	74226
Ion Ratio	Lower	Upper	
212	100		
106	12.8	9.8	14.6
104	7.2	5.4	8.2

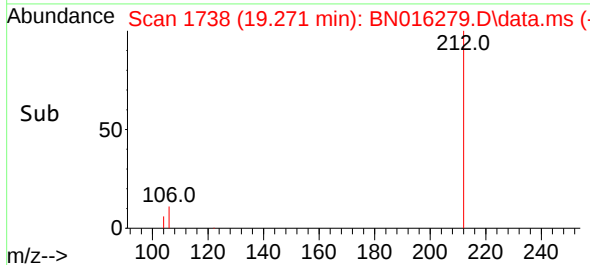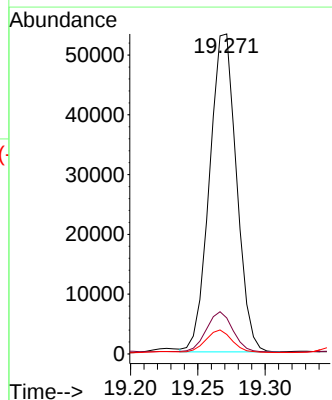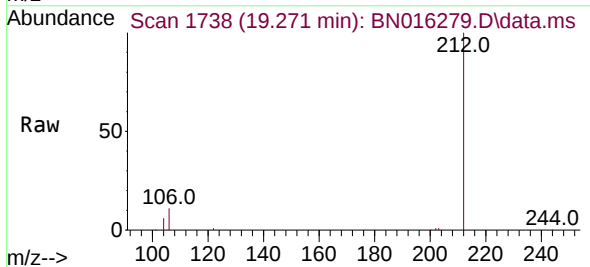

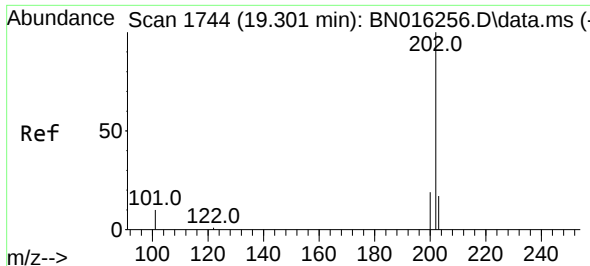





#28
Fluoranthene
Concen: 0.026 ng
RT: 19.296 min Scan# 1743
Delta R.T. -0.005 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion:202 Resp: 6500
Ion Ratio Lower Upper
202 100
101 12.4 8.5 12.7
203 22.2 13.8 20.8#

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

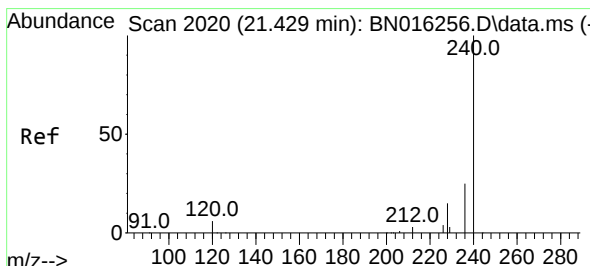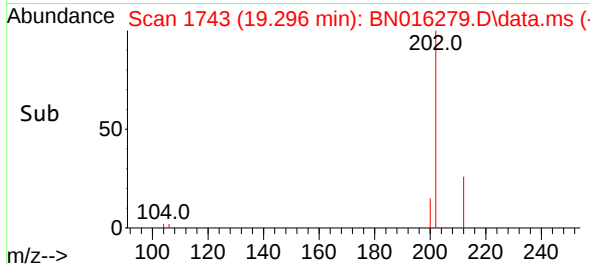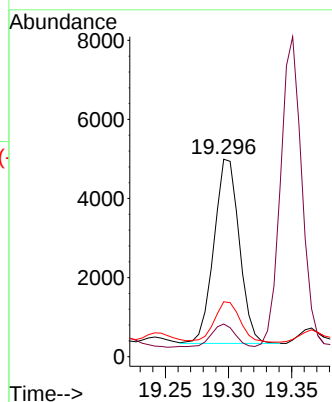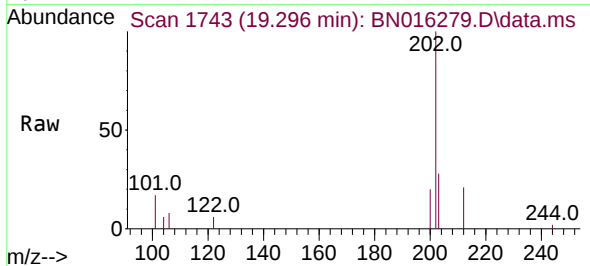

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.429 min Scan# 2020
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion:240 Resp: 69928
Ion Ratio Lower Upper
240 100
120 5.3 5.3 7.9
236 24.2 19.8 29.8

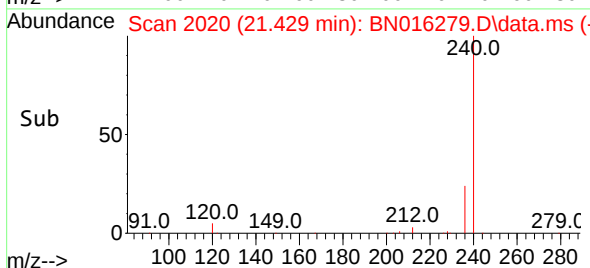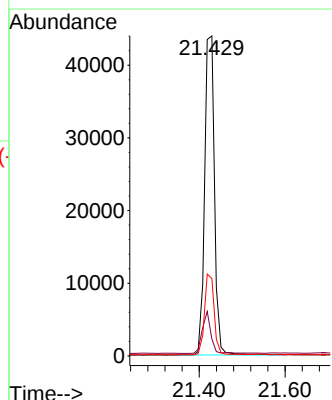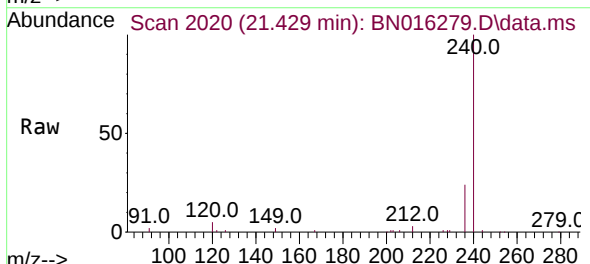

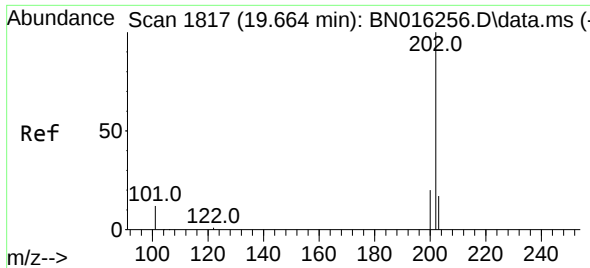





#30
Pyrene
Concen: 0.054 ng
RT: 19.664 min Scan# 1817
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

Tgt Ion:202 Resp: 12784
Ion Ratio Lower Upper
202 100
200 18.9 15.8 23.6
203 42.7 13.9 20.9#

Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642




Manual Integrations
APPROVED


mohammad
9/10/2021 3:24:04 PM

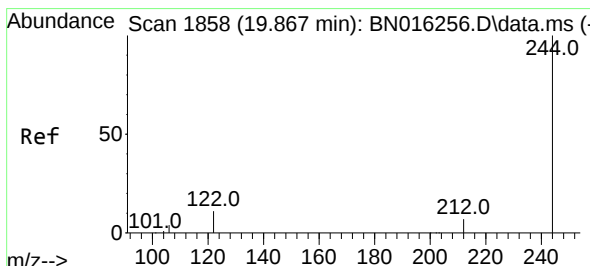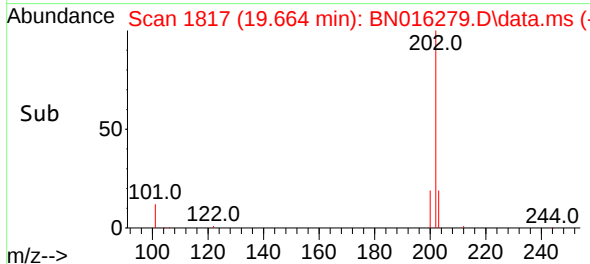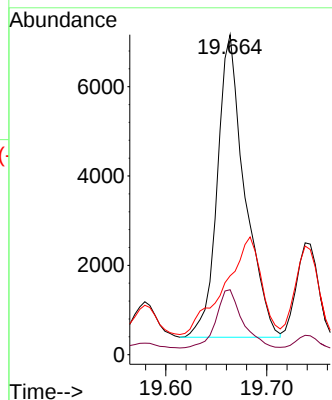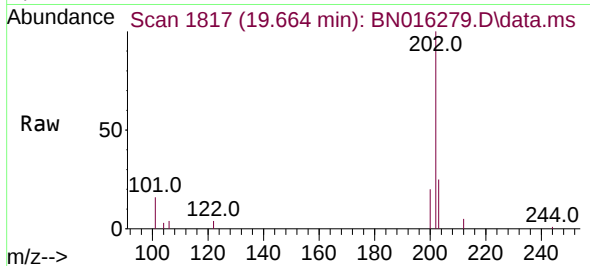

#31
Terphenyl-d14
Concen: 0.403 ng
RT: 19.867 min Scan# 1858
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44


Tgt Ion:244 Resp: 70770
Ion Ratio Lower Upper
244 100
212 6.8 5.5 8.3
122 9.9 9.0 13.4

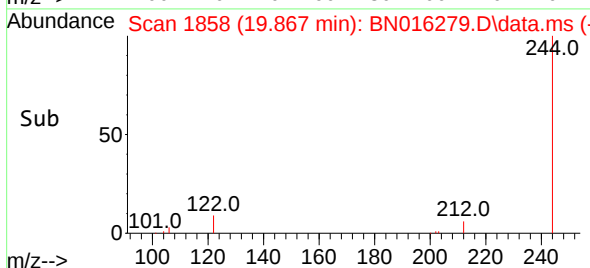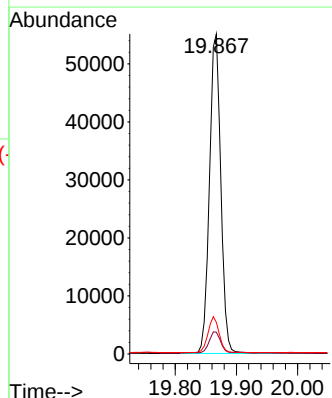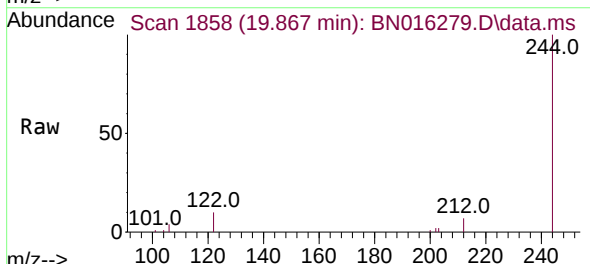

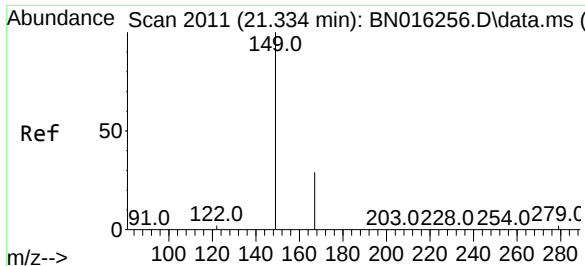

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.289 ng
RT: 21.334 min Scan# 2011
Delta R.T. -0.000 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44



Instrument :
BNA_N
ClientSampleId :
BP-TT-VPB-RW7-GW-640-642

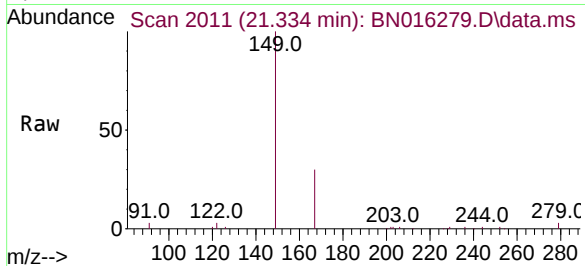


Tgt Ion:149 Resp: 38748
Ion Ratio Lower Upper
149 100
167 28.5 23.4 35.0
279 4.7 3.9 5.9

Manual Integrations
APPROVED

mohammad
9/10/2021 3:24:04 PM

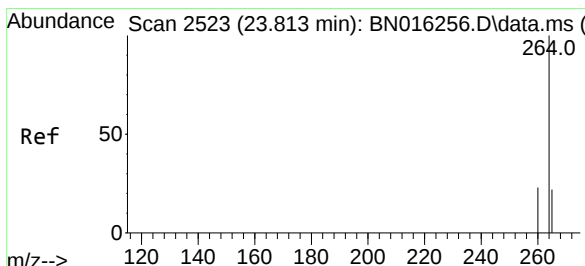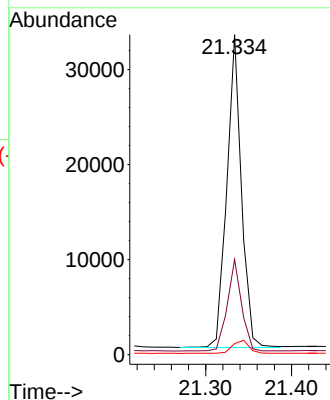

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.810 min Scan# 2522
Delta R.T. -0.003 min
Lab File: BN016279.D
Acq: 10 Sep 2021 05:44

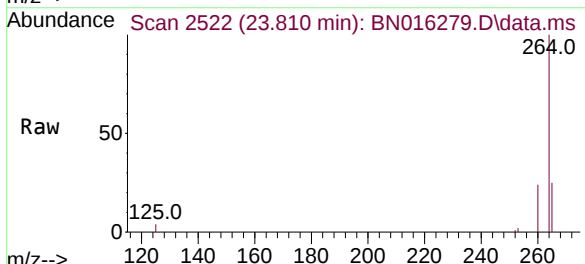

Tgt Ion:264 Resp: 47932
Ion Ratio Lower Upper
264 100
260 23.7 18.9 28.3
265 25.4 23.7 35.5

