
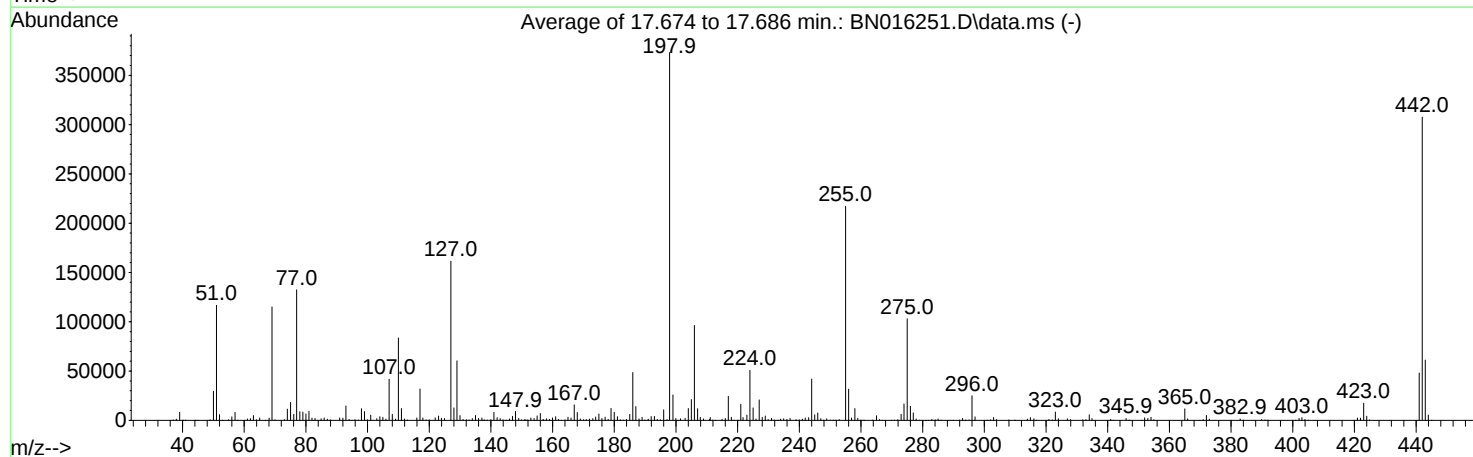


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
 Data File : BN016251.D
 Acq On : 09 Sep 2021 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 10 14:34:37 2021

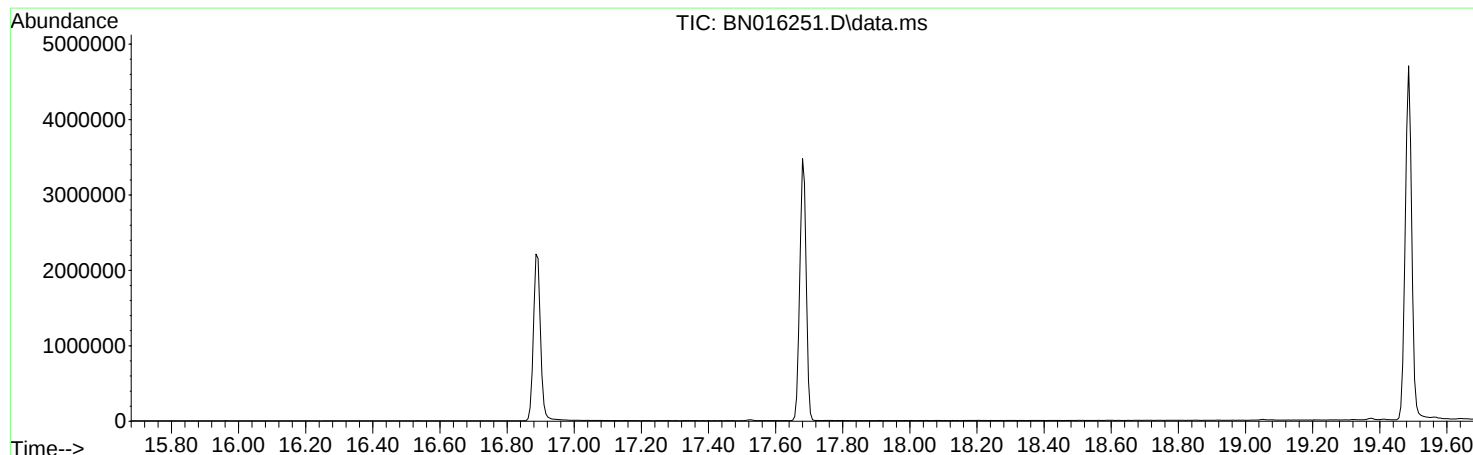

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.3	116731	PASS
68	69	0.00	2	1.9	2216	PASS
69	198	0.00	100	30.8	115043	PASS
70	69	0.00	2	0.5	584	PASS
127	198	10	80	43.3	161472	PASS
197	198	0.00	2	0.2	812	PASS
198	198	100	100	100.0	373141	PASS
199	198	5	9	6.9	25752	PASS
275	198	10	60	27.6	103056	PASS
365	198	1	100	3.1	11648	PASS
441	198	0.01	100	12.9	47992	PASS
442	442	50	100	100.0	307605	PASS
443	442	15	24	19.9	61149	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/9/2021	BNA_N	<u>BN016251.D</u>
Compound Name	Response	Retention Time
DDT	1306355	20.721
DDD	110541	20.28
DDE	10158	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
120699	1427054	8.46

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
 Data File : BN016251.D
 Acq On : 09 Sep 2021 10:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 09 11:27:50 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 17:12:56 2021
 Response via : Initial Calibration

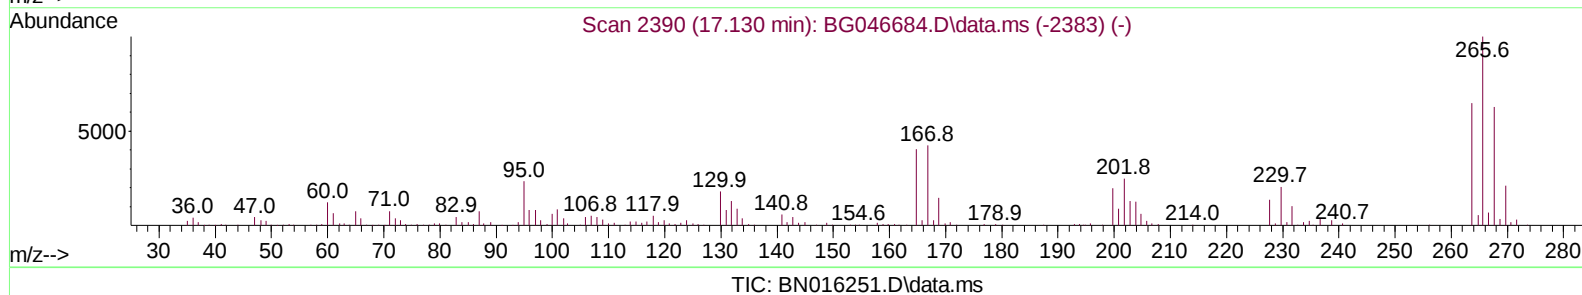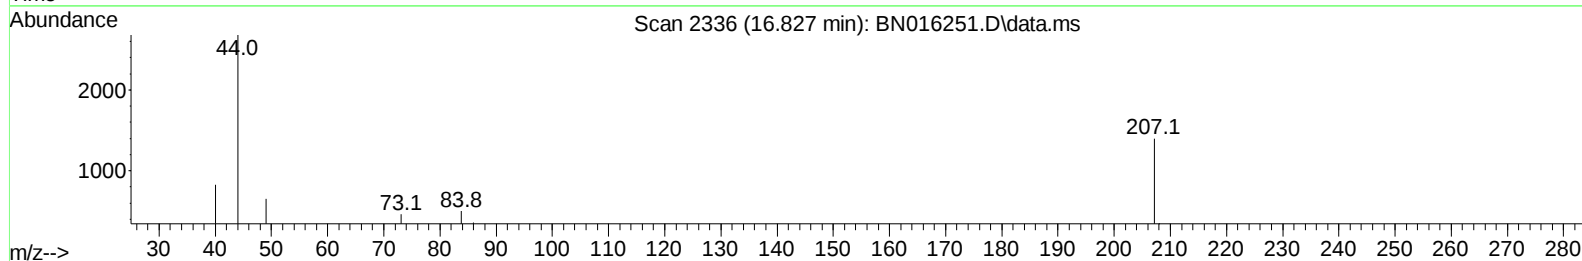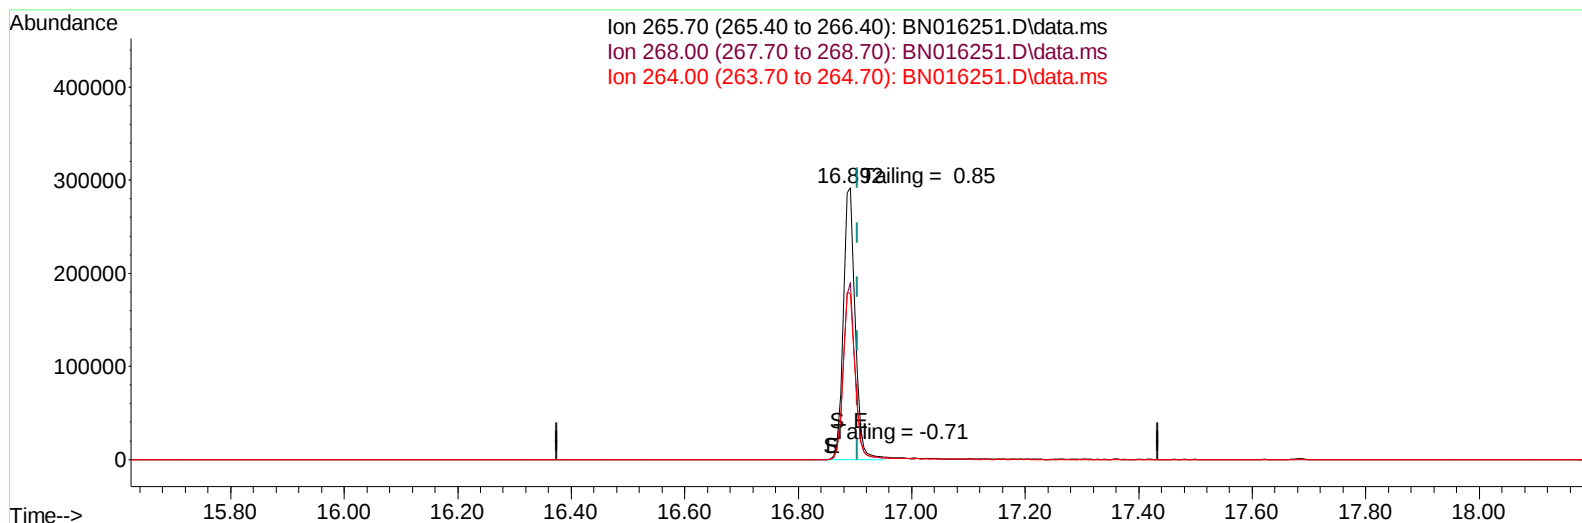

(70) Pentachlorophenol (C)




16.892min (-0.012) 21743.19 ng m

response 390413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.28
264.00	61.60	61.01
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 09 11:27:50 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

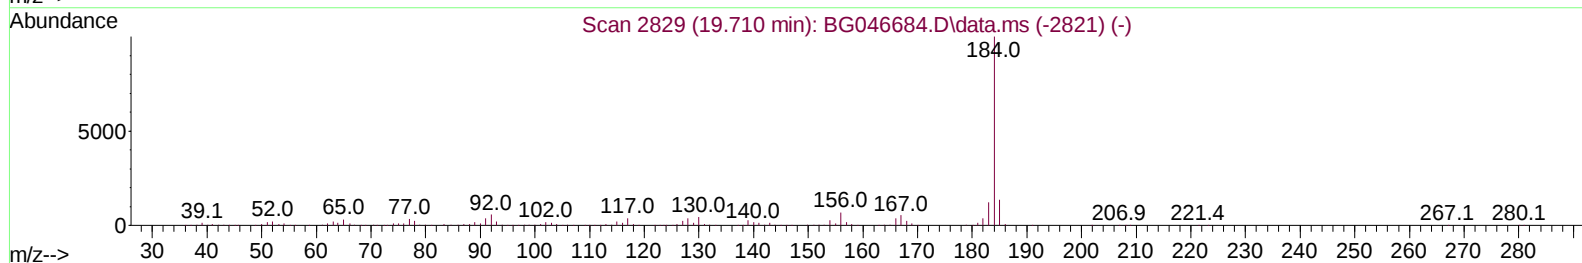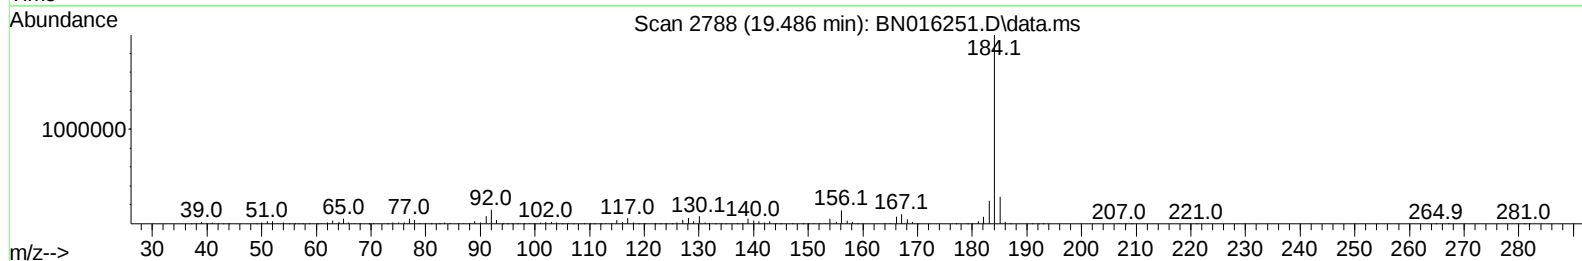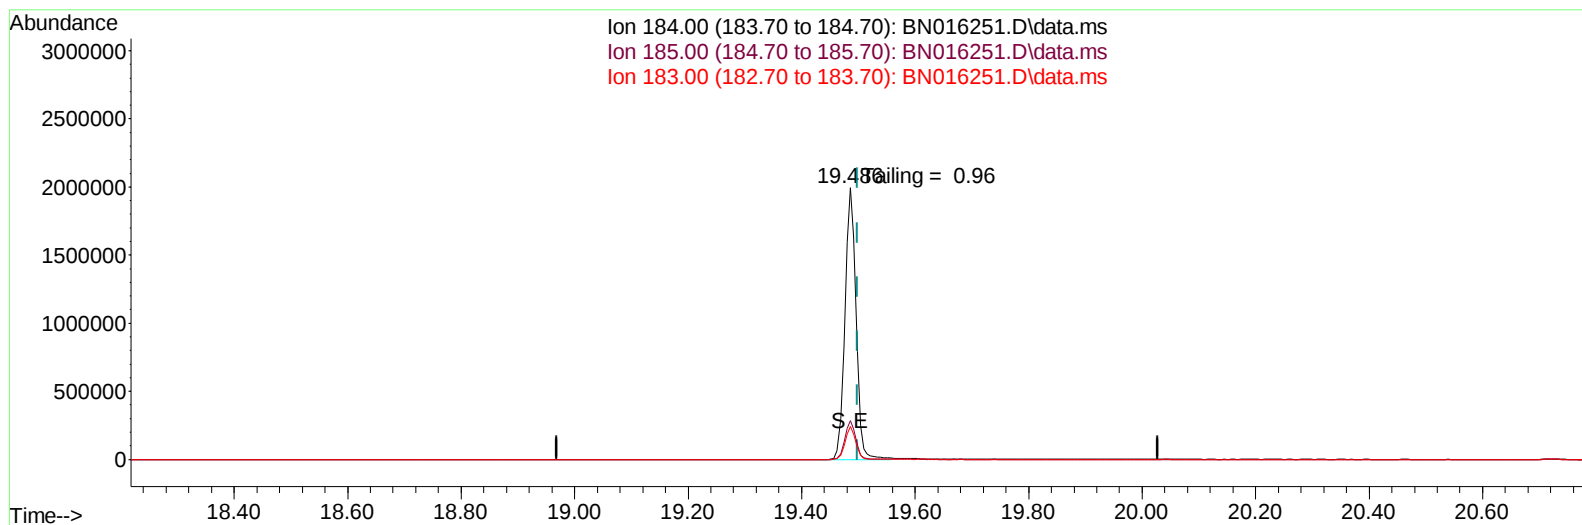

TIC: BN016251.D\data.ms

(77) Benzidine

19.486min (-0.012) 0.00 ng

response **2748358**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	12.14
0.00	0.00	0.00