
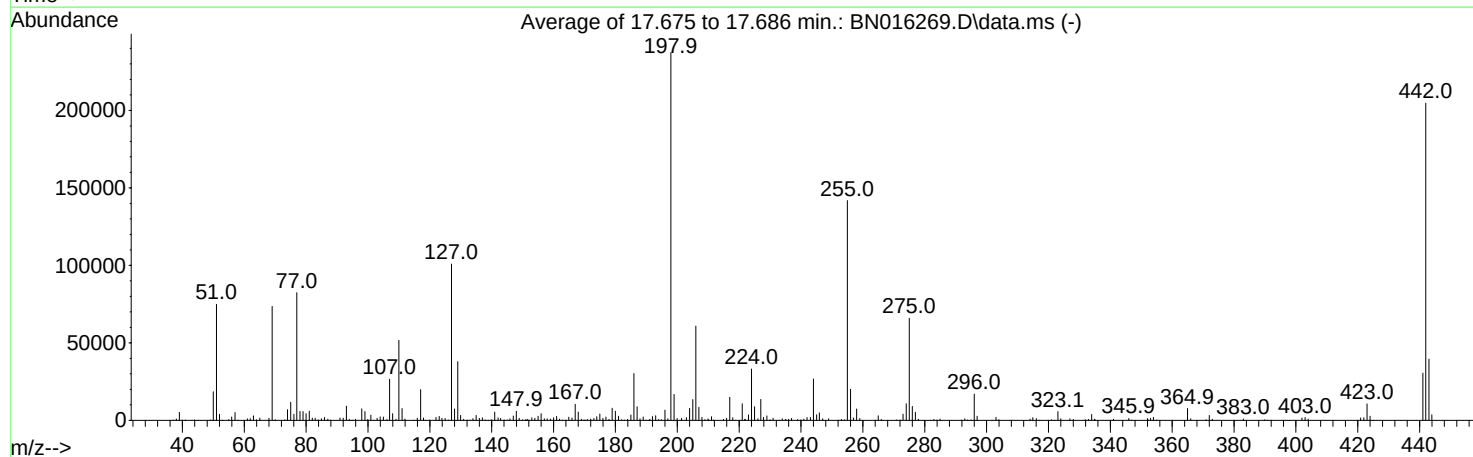


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
 Data File : BN016269.D
 Acq On : 09 Sep 2021 22:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 10 14:34:37 2021

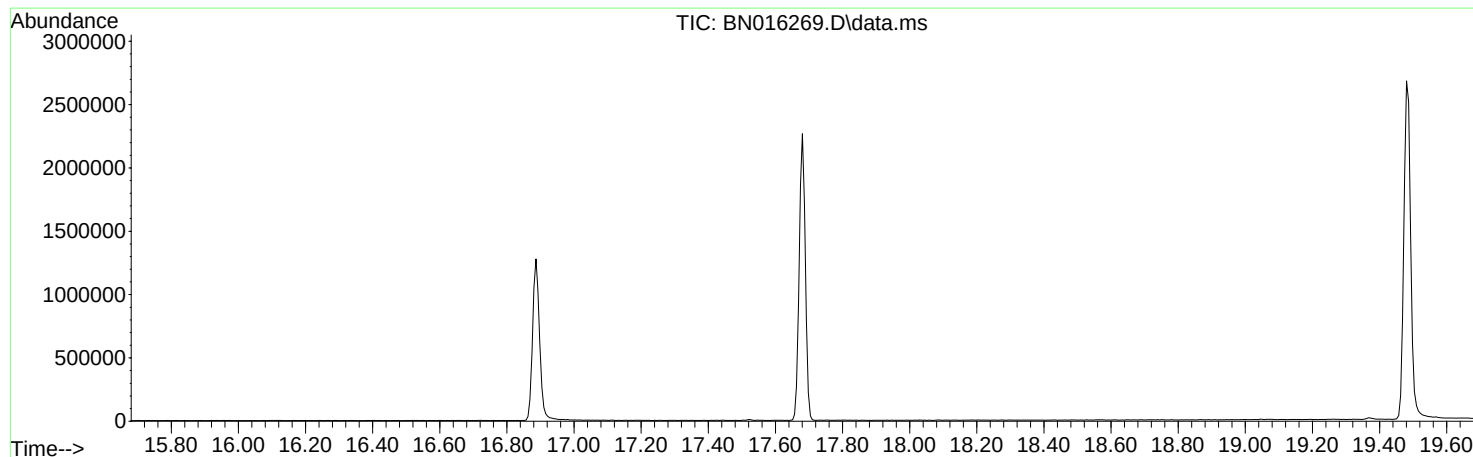

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	74848	PASS
68	69	0.00	2	1.8	1322	PASS
69	198	0.00	100	31.0	73536	PASS
70	69	0.00	2	0.5	374	PASS
127	198	10	80	42.5	100843	PASS
197	198	0.00	2	0.4	990	PASS
198	198	100	100	100.0	237355	PASS
199	198	5	9	7.0	16681	PASS
275	198	10	60	27.8	65872	PASS
365	198	1	100	3.2	7629	PASS
441	198	0.01	100	12.8	30416	PASS
442	442	50	100	100.0	204757	PASS
443	442	15	24	19.3	39531	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/9/2021	BNA_N	<u>BN016269.D</u>
Compound Name	Response	Retention Time
DDT	765169	20.721
DDD	76258	20.28
DDE	5958	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
82216	847385	9.70

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016269.D
Acq On : 09 Sep 2021 22:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 02:37:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

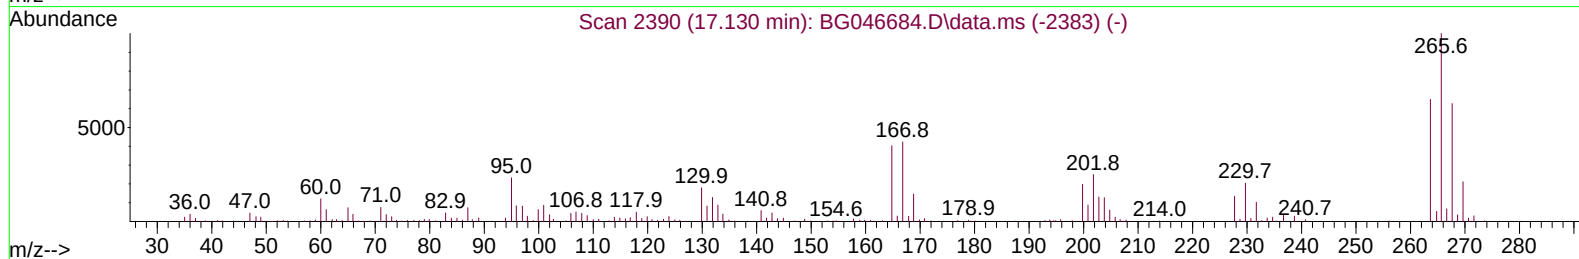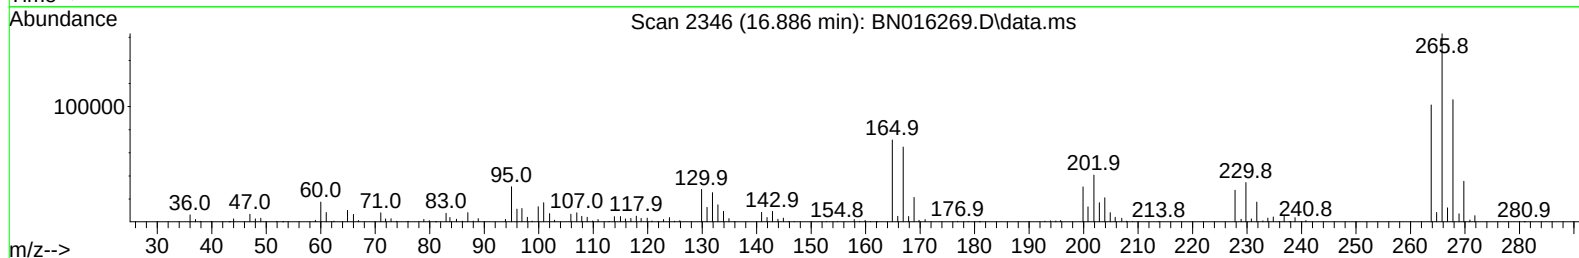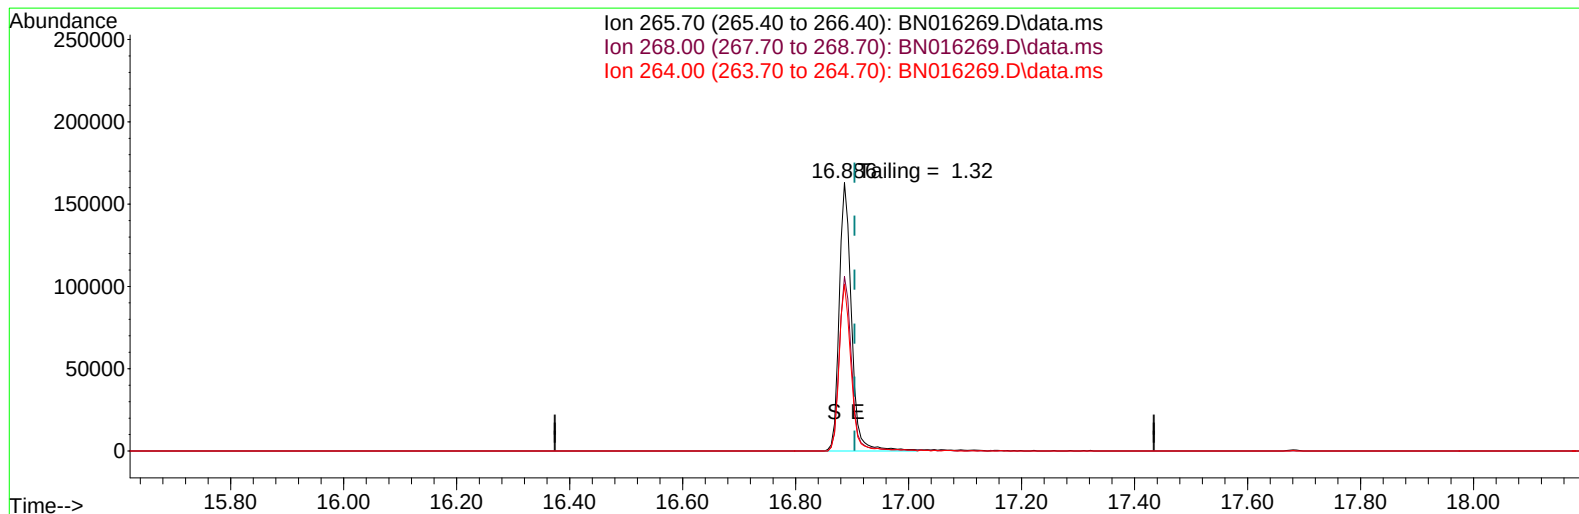

TIC: BN016269.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.018) 21322.32 ng




response 244305

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.98
264.00	61.60	62.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016269.D
Acq On : 09 Sep 2021 22:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 02:37:40 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

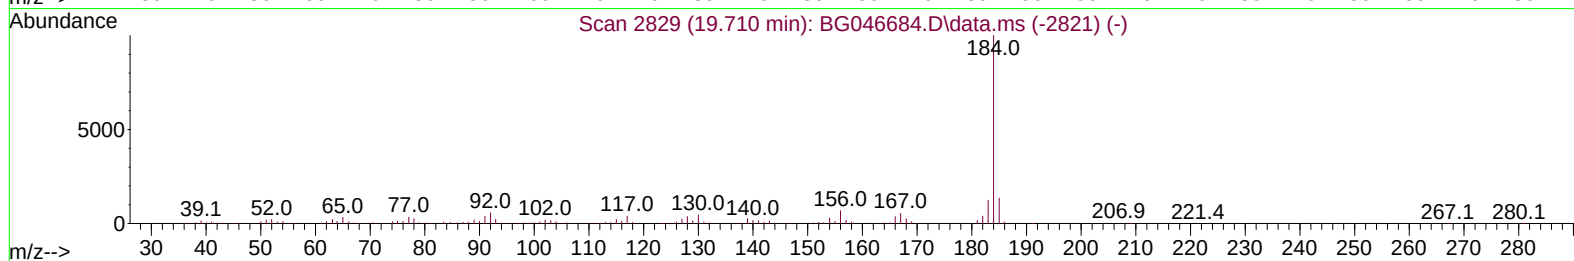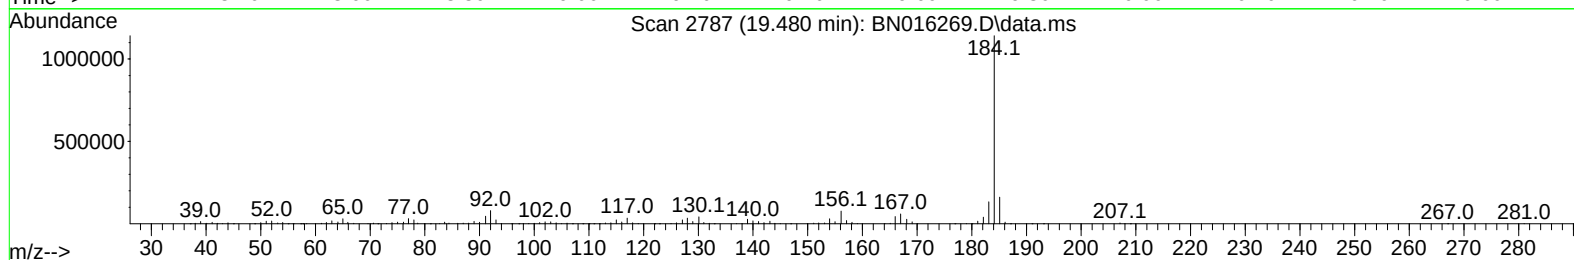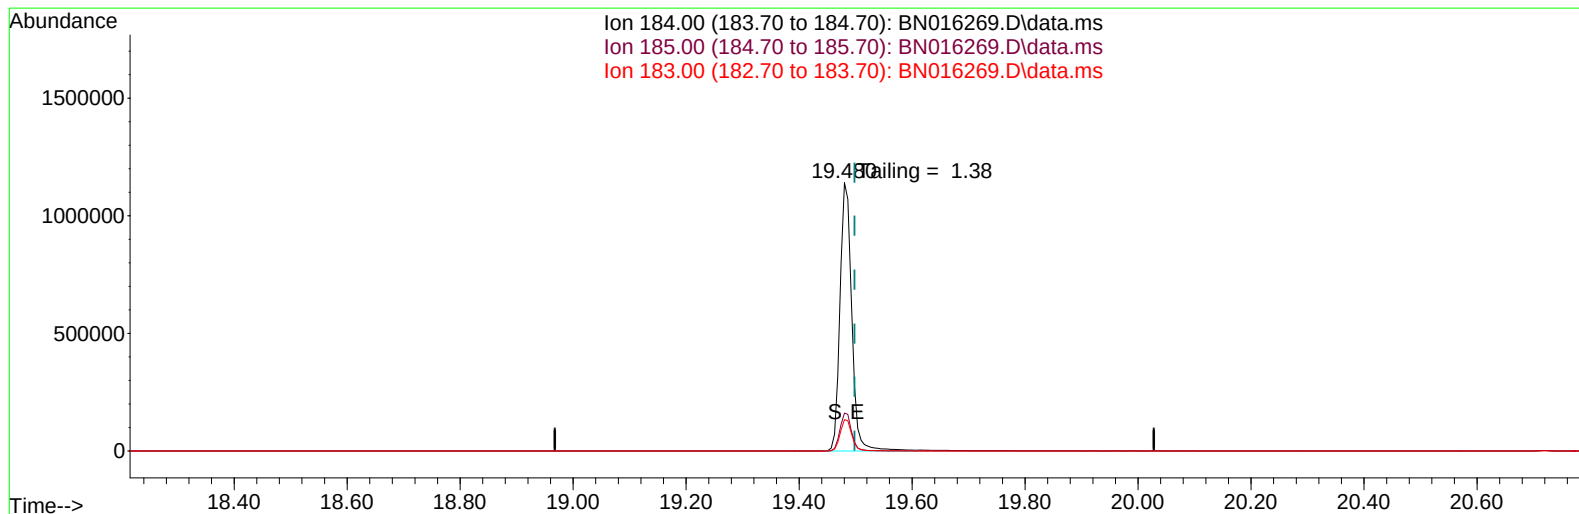

TIC: BN016269.D\data.ms

(77) Benzidine

19.480min (-0.018) 0.00 ng

response 1641515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.15
183.00	13.20	11.73
0.00	0.00	0.00