
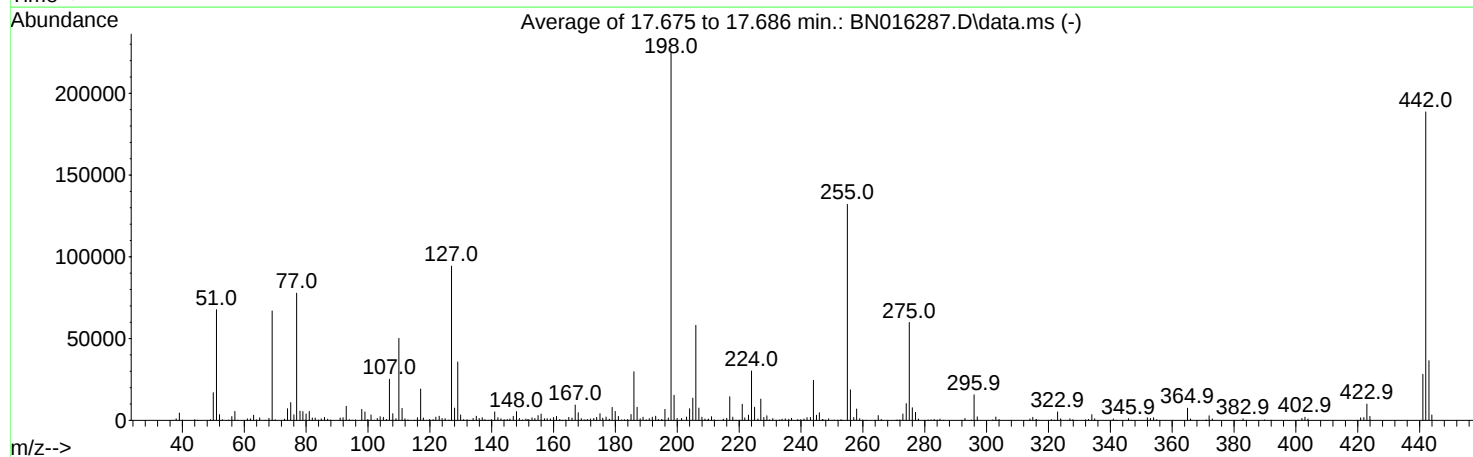


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
 Data File : BN016287.D
 Acq On : 10 Sep 2021 10:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN090921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 10 14:34:37 2021

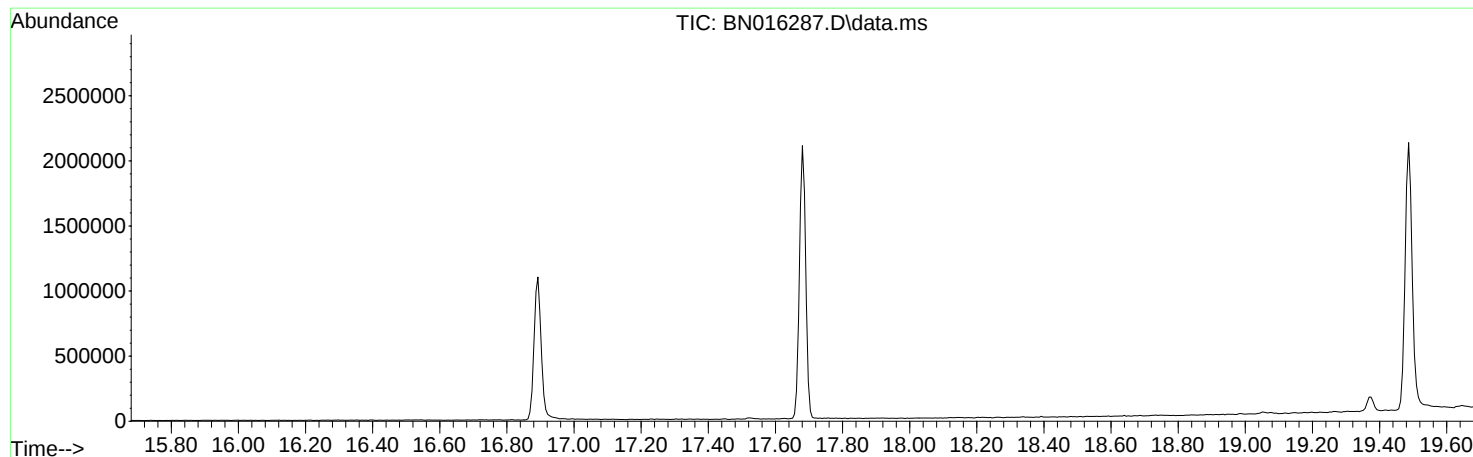

AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	67709	PASS
68	69	0.00	2	1.9	1284	PASS
69	198	0.00	100	29.7	66923	PASS
70	69	0.00	2	0.6	427	PASS
127	198	10	80	41.9	94317	PASS
197	198	0.00	2	0.6	1461	PASS
198	198	100	100	100.0	224960	PASS
199	198	5	9	6.8	15377	PASS
275	198	10	60	26.6	59840	PASS
365	198	1	100	3.3	7437	PASS
441	198	0.01	100	12.5	28232	PASS
442	442	50	100	100.0	188608	PASS
443	442	15	24	19.4	36523	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/9/2021	BNA_N	<u>BN016287.D</u>
Compound Name	Response	Retention Time
DDT	715784	20.721
DDD	89540	20.28
DDE	13735	19.774
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
103275	819059	12.61

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016287.D
Acq On : 10 Sep 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 13:00:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

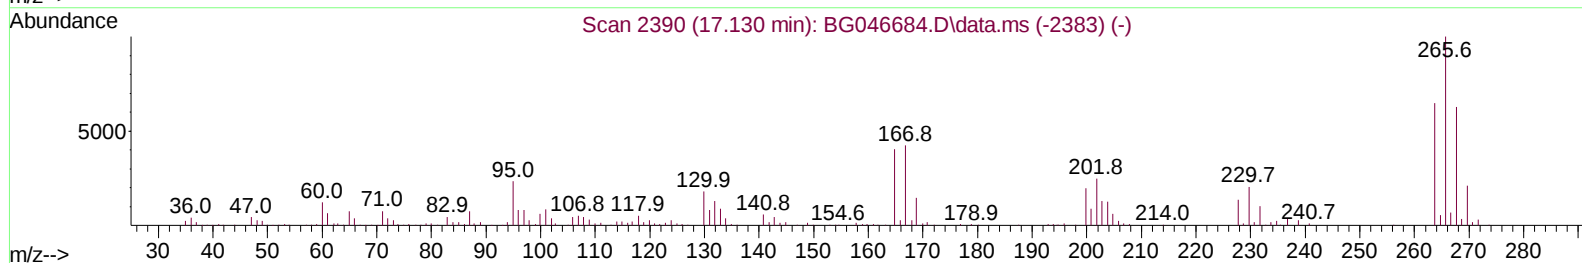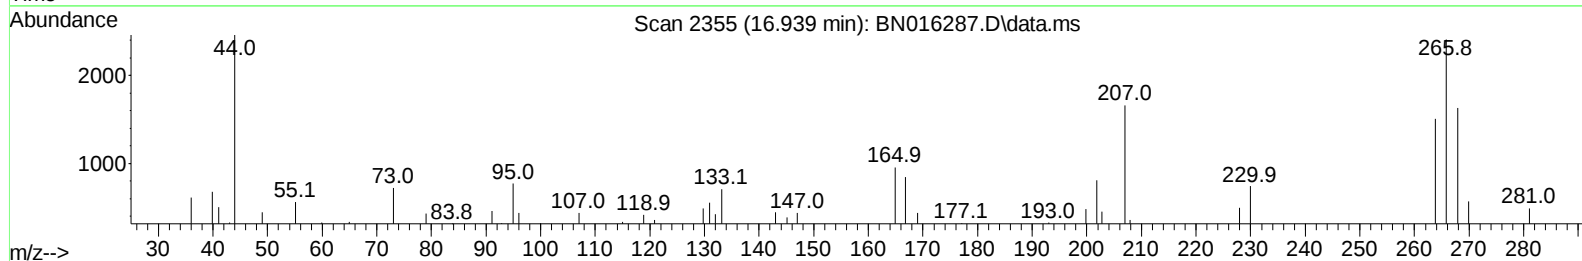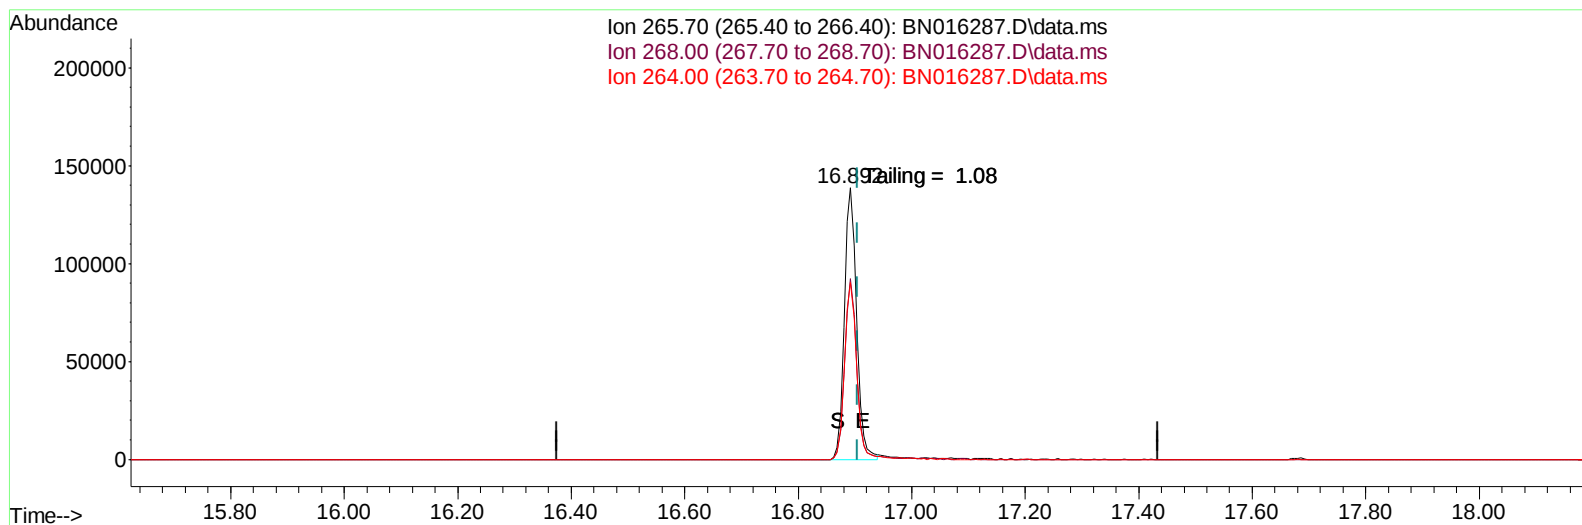

TIC: BN016287.D\data.ms

(70) Pentachlorophenol (C)

16.939min (+ 0.035) 137.17 ng m




response 1379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.73
264.00	61.60	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090921\
Data File : BN016287.D
Acq On : 10 Sep 2021 10:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 10 13:00:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 17:12:56 2021
Response via : Initial Calibration

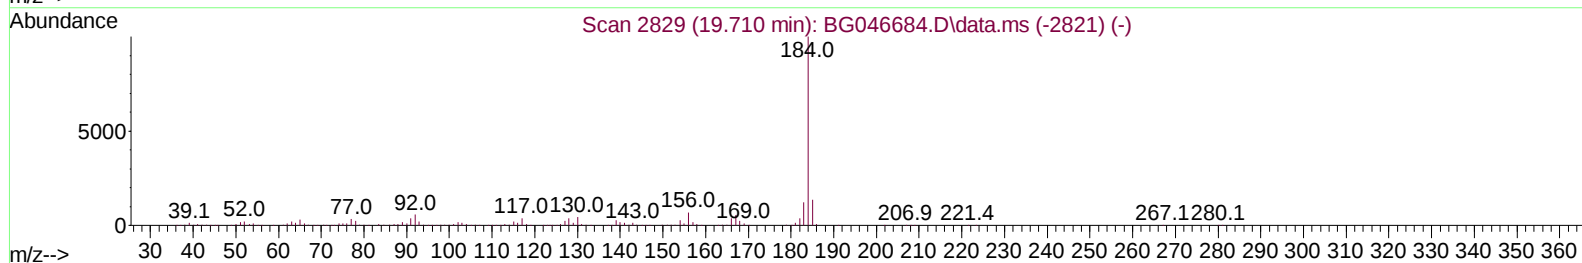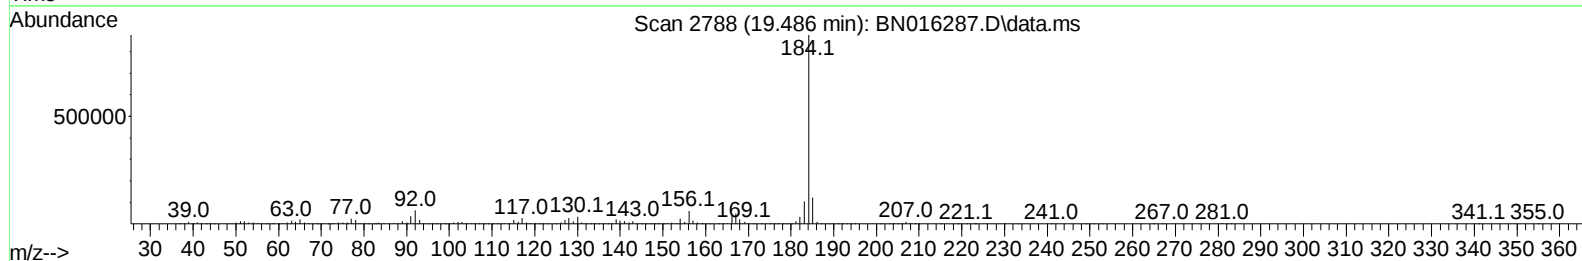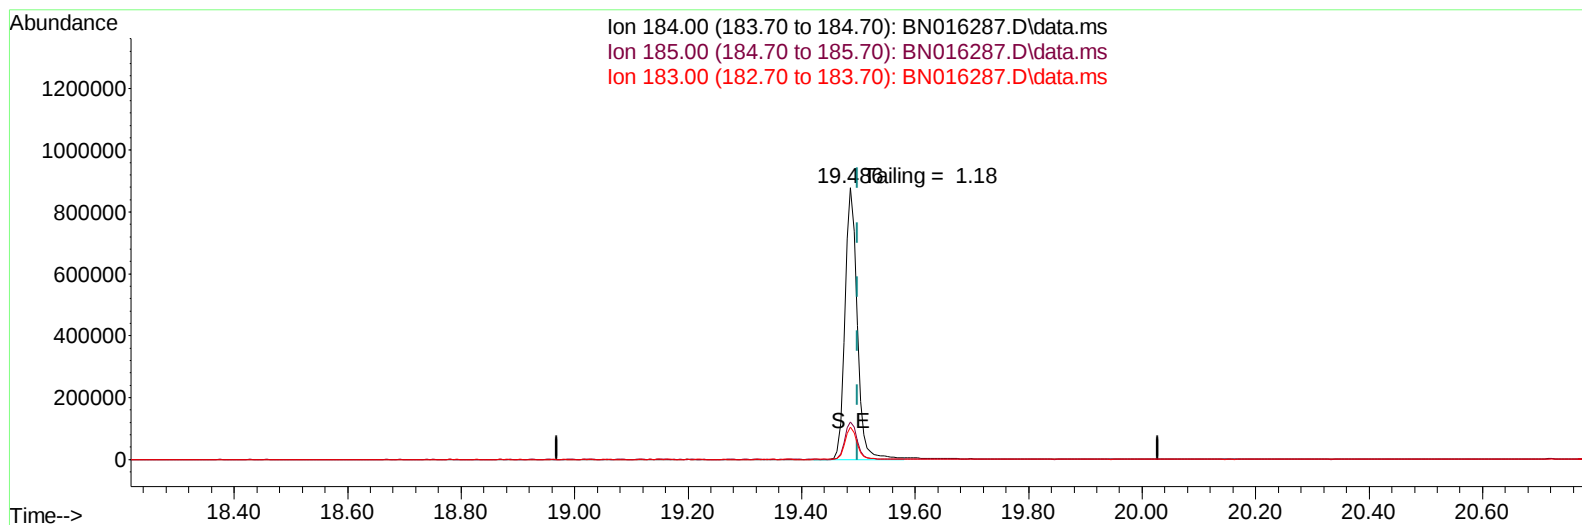

TIC: BN016287.D\data.ms

(77) Benzidine

19.486min (-0.012) 41434.32 ng

response 1320654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.94
0.00	0.00	0.00