

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027496.D
 Acq On : 09 Sep 2023 11:38
 Operator : MA/JU
 Sample : PB155273BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK273

Quant Time: Sep 10 00:09:42 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	9018	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	30702	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164	19172	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	43309	0.400	ng/ul	0.00
17) Chrysene-d12	21.598	240	33268	0.400	ng/ul	0.00
23) Perylene-d12	24.103	264	33526	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	58367	4.866	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	13188	0.283	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	33080	0.290	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.665	166	4802	0.057	ng/ul#	13
20) Pyrene	19.813	202	4460	0.029	ng/ul#	1
26) Benzo(a)pyrene	23.942	252	9008	0.073	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027496.D
Acq On : 09 Sep 2023 11:38
Operator : MA/JU
Sample : PB155273BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK273

Quant Time: Sep 10 00:09:42 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

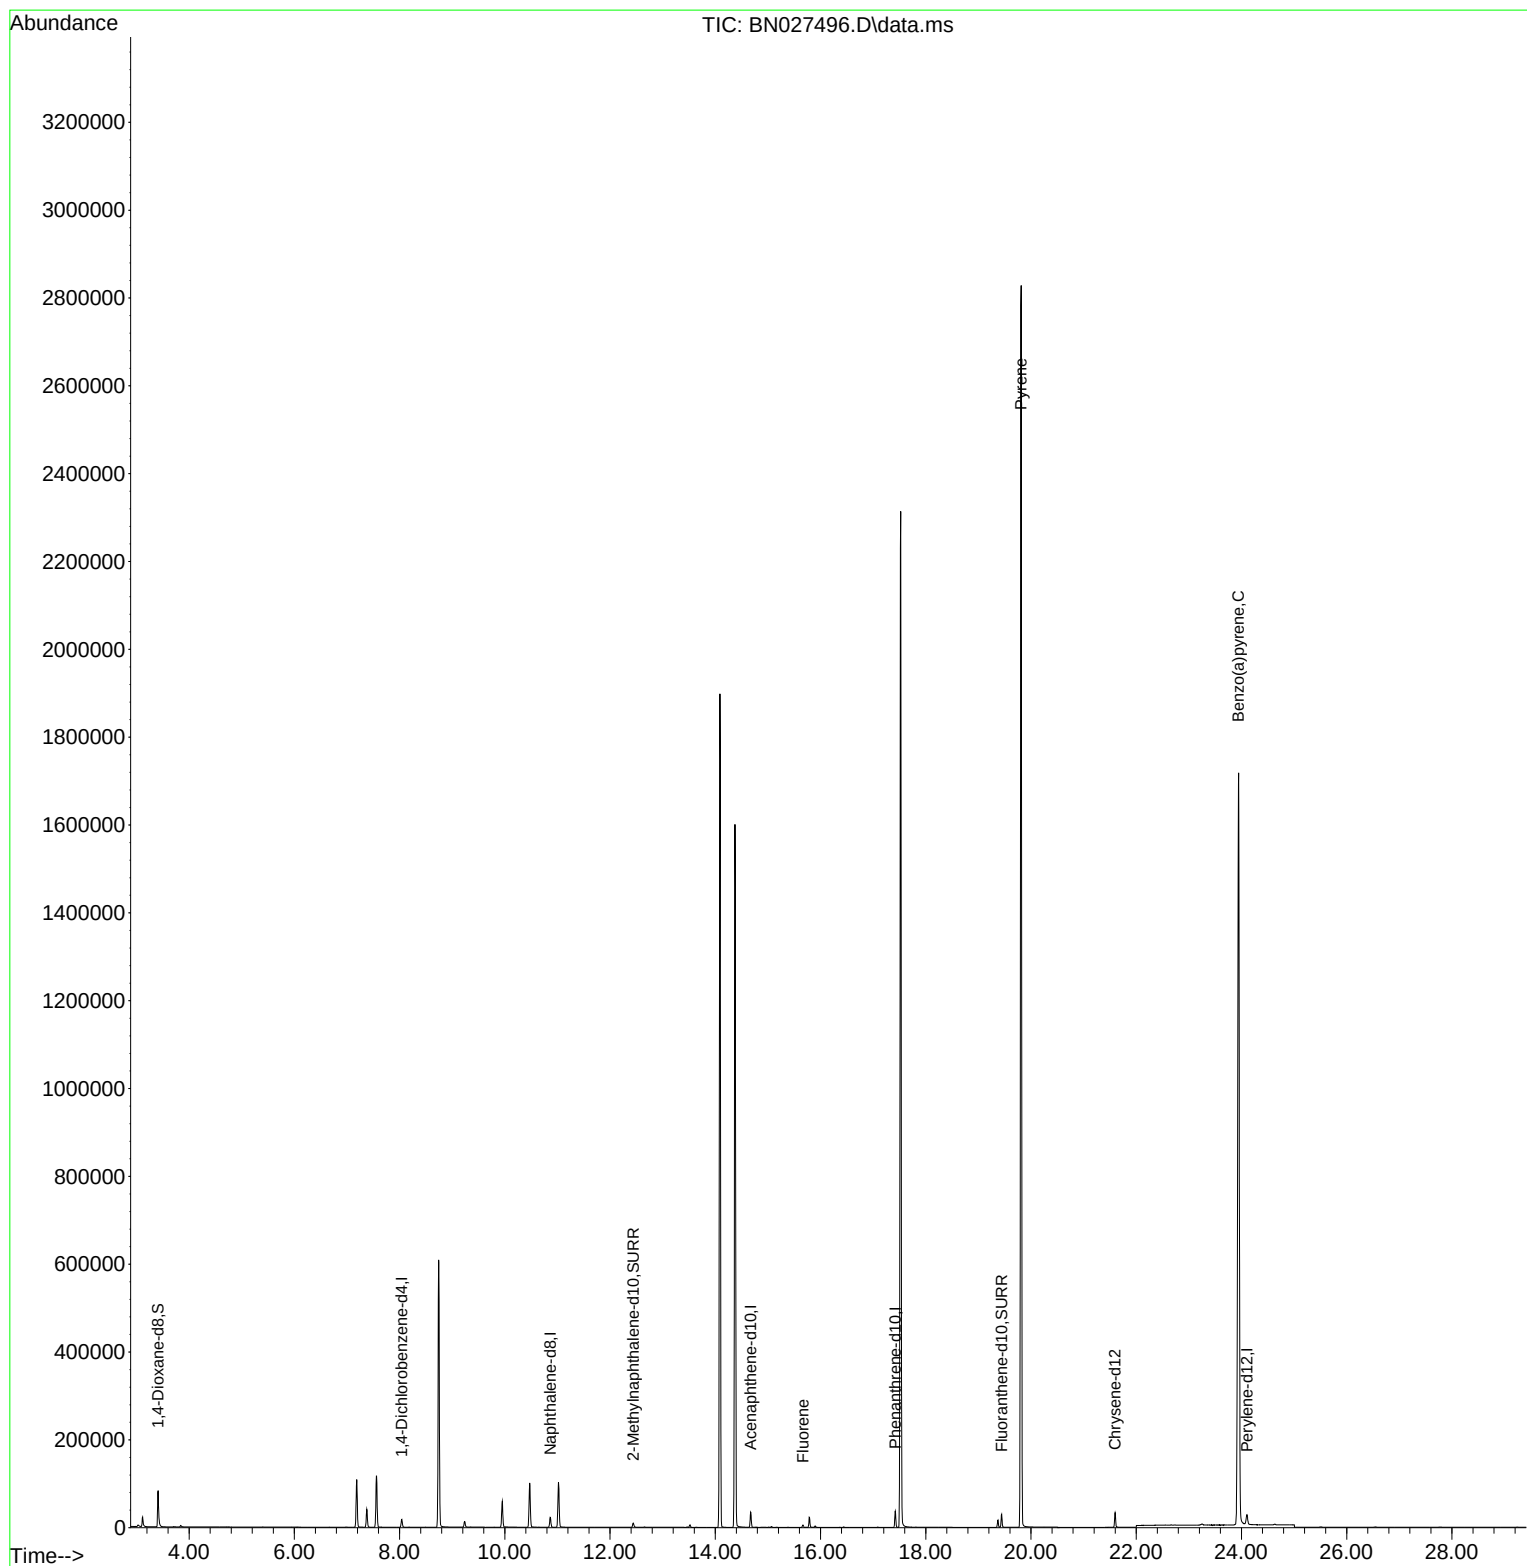

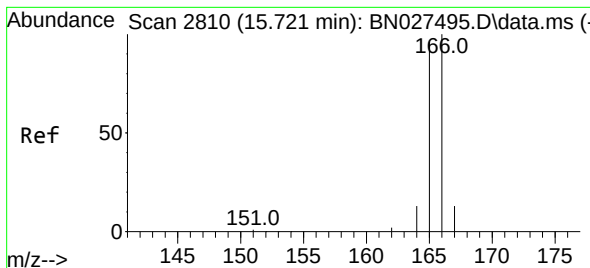

#12

Fluorene

Concen: 0.057 ng/ul

RT: 15.665 min Scan# 21

Delta R.T. -0.060 min

Lab File: BN027496.D

Acq: 09 Sep 2023 11:38

Instrument :

BNA_N

ClientSampleId :

SBLK273





Tgt Ion:166 Resp: 4802

Ion Ratio Lower Upper

166 100

165 7.3 79.6 119.4#

167 33.6 11.4 17.0#

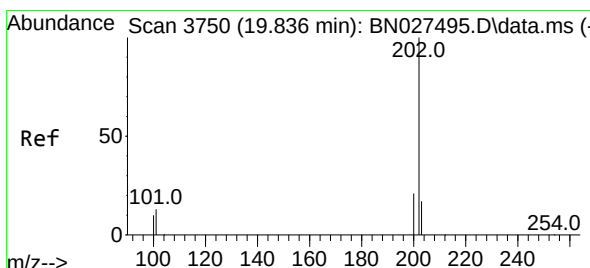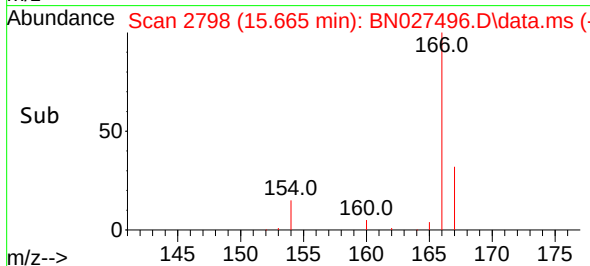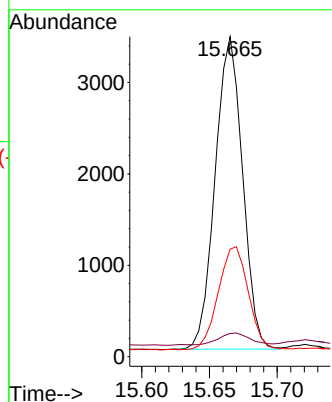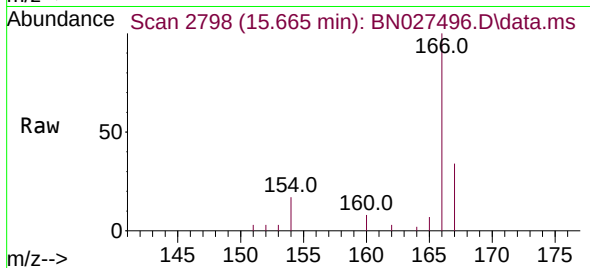

#20

Pyrene

Concen: 0.029 ng/ul

RT: 19.813 min Scan# 3745

Delta R.T. -0.028 min

Lab File: BN027496.D

Acq: 09 Sep 2023 11:38




Tgt Ion:202 Resp: 4460


Ion Ratio Lower Upper

202 100

101 145.6 11.4 17.2#


100 1044.3 9.4 14.2#

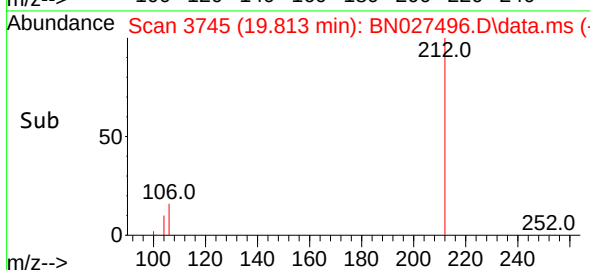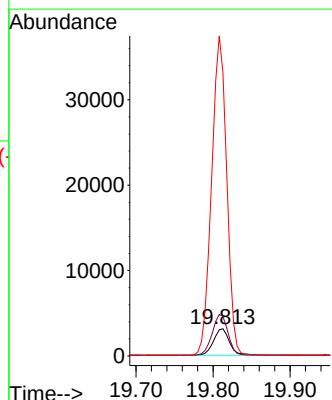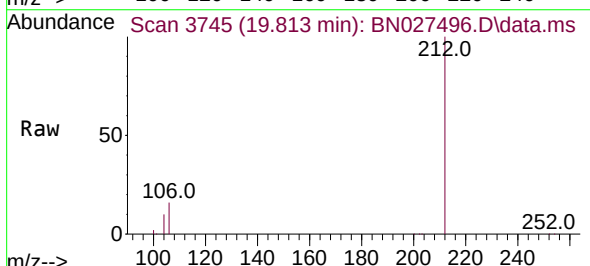

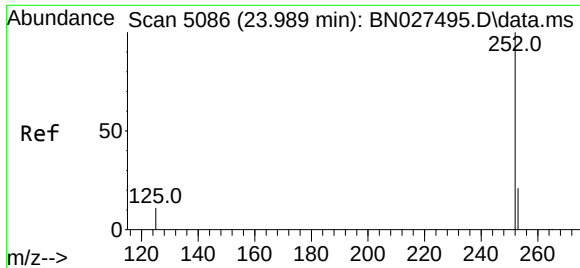

#26
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.942 min Scan# 50
Delta R.T. -0.053 min
Lab File: BN027496.D
Acq: 09 Sep 2023 11:38

Instrument :
BNA_N
ClientSampleId :
SBLK273

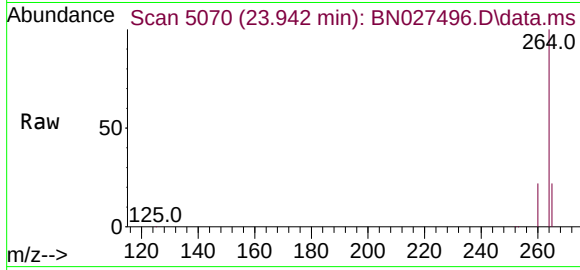

Tgt Ion:252 Resp: 9008
Ion Ratio Lower Upper
252 100
253 43.3 22.4 33.6#
125 37.6 17.4 26.2#

