

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027497.D
 Acq On : 09 Sep 2023 12:15
 Operator : MA/JU
 Sample : PB155239BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK239

Quant Time: Sep 10 00:09:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	13632	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	47640	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.675	164	29752	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.421	188	65244	0.400	ng/ul	0.00
17) Chrysene-d12	21.597	240	49177	0.400	ng/ul	# 0.00
23) Perylene-d12	24.102	264	47809	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	82479	4.548	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	21535	0.298	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	52298	0.310	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.670	166	7191	0.055	ng/ul#	11
20) Pyrene	19.812	202	6462	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.944	252	13256	0.075	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027497.D
Acq On : 09 Sep 2023 12:15
Operator : MA/JU
Sample : PB155239BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK239

Quant Time: Sep 10 00:09:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




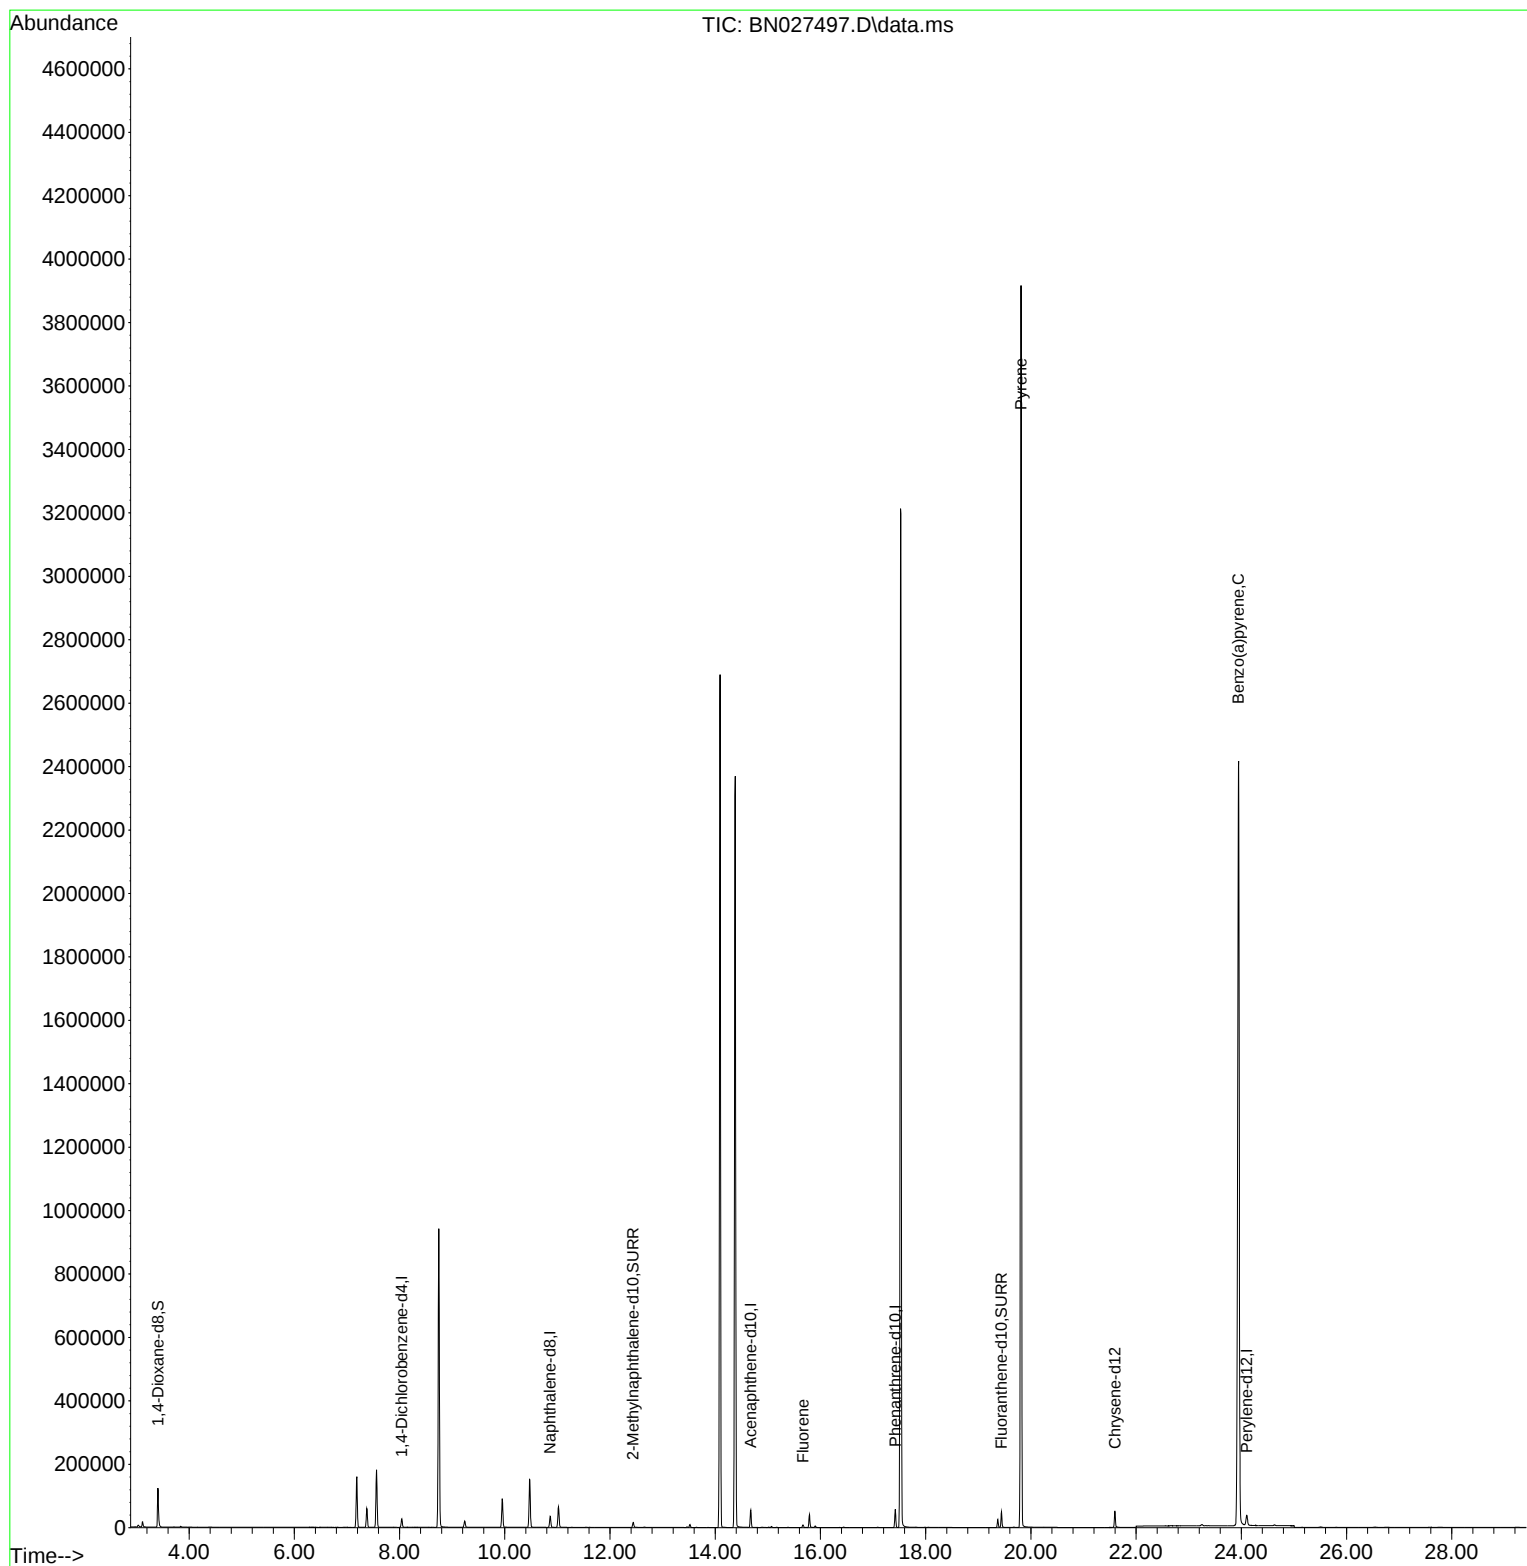


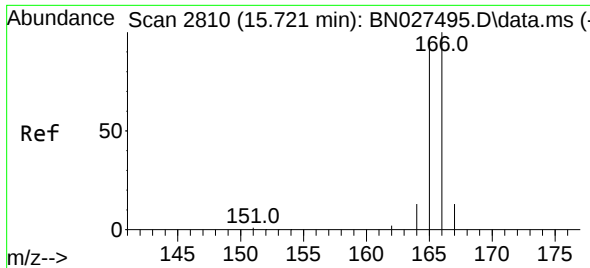

#12
Fluorene
Concen: 0.055 ng/ul
RT: 15.670 min Scan# 21
Delta R.T. -0.056 min
Lab File: BN027497.D
Acq: 09 Sep 2023 12:15




Instrument :
BNA_N
ClientSampleId :
SBLK239


Tgt Ion:166 Resp: 7191
Ion Ratio Lower Upper
166 100
165 6.0 79.6 119.4#
167 35.5 11.4 17.0#

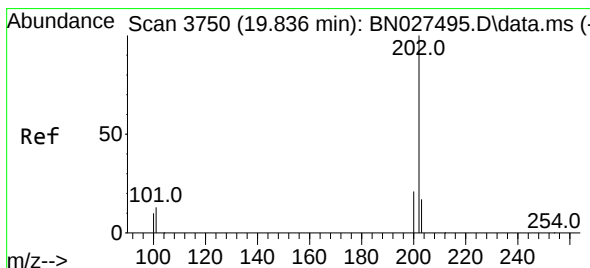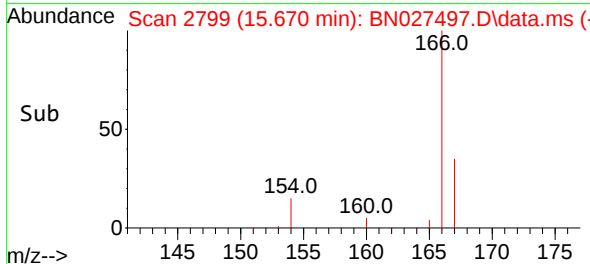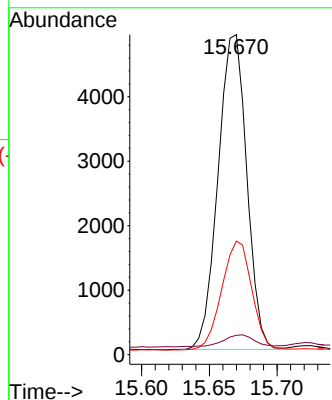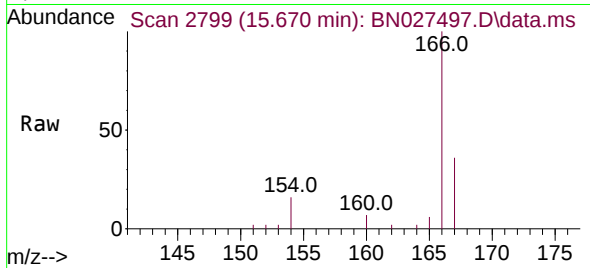

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.812 min Scan# 3745
Delta R.T. -0.028 min
Lab File: BN027497.D
Acq: 09 Sep 2023 12:15


Tgt Ion:202 Resp: 6462
Ion Ratio Lower Upper
202 100
101 147.8 11.4 17.2#
100 1098.6 9.4 14.2#

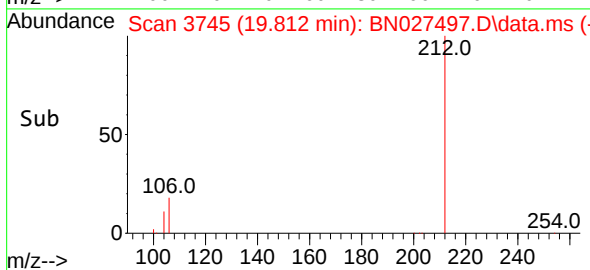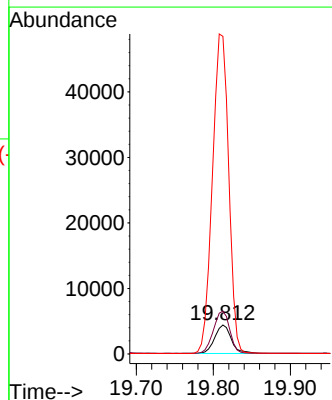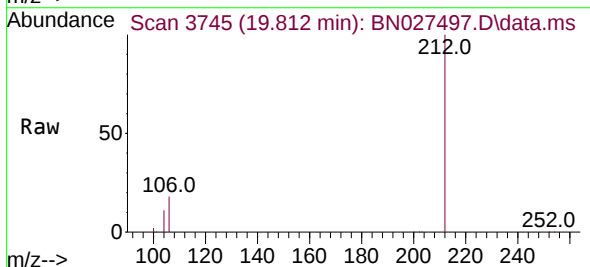

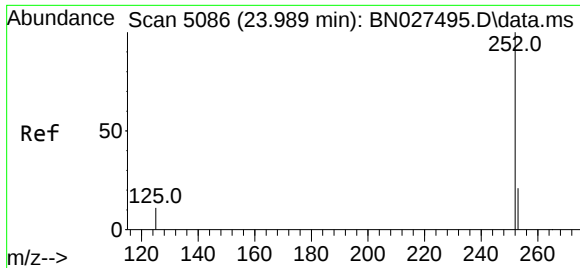

#26
Benzo(a)pyrene
Concen: 0.075 ng/ul
RT: 23.944 min Scan# 50
Delta R.T. -0.050 min
Lab File: BN027497.D
Acq: 09 Sep 2023 12:15

Instrument :
BNA_N
ClientSampleId :
SBLK239

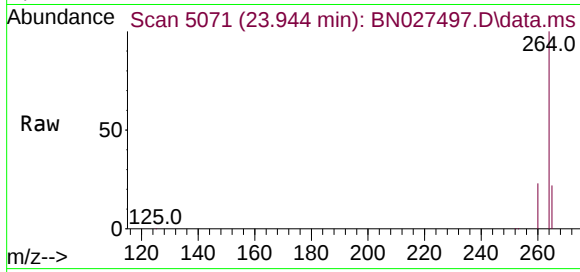

Tgt Ion:252 Resp: 13256
Ion Ratio Lower Upper
252 100
253 39.3 22.4 33.6#
125 31.3 17.4 26.2#

