

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027498.D
 Acq On : 09 Sep 2023 12:52
 Operator : MA/JU
 Sample : PB155241BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK241

Quant Time: Sep 10 00:10:04 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	9578	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	33250	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.675	164	20813	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	45455	0.400	ng/ul	0.00
17) Chrysene-d12	21.598	240	34668	0.400	ng/ul	0.00
23) Perylene-d12	24.109	264	34383	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	78998	6.200	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	20479	0.406	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	50332	0.424	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.813	202	6922	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.951	252	13384	0.106	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027498.D
Acq On : 09 Sep 2023 12:52
Operator : MA/JU
Sample : PB155241BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK241

Quant Time: Sep 10 00:10:04 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

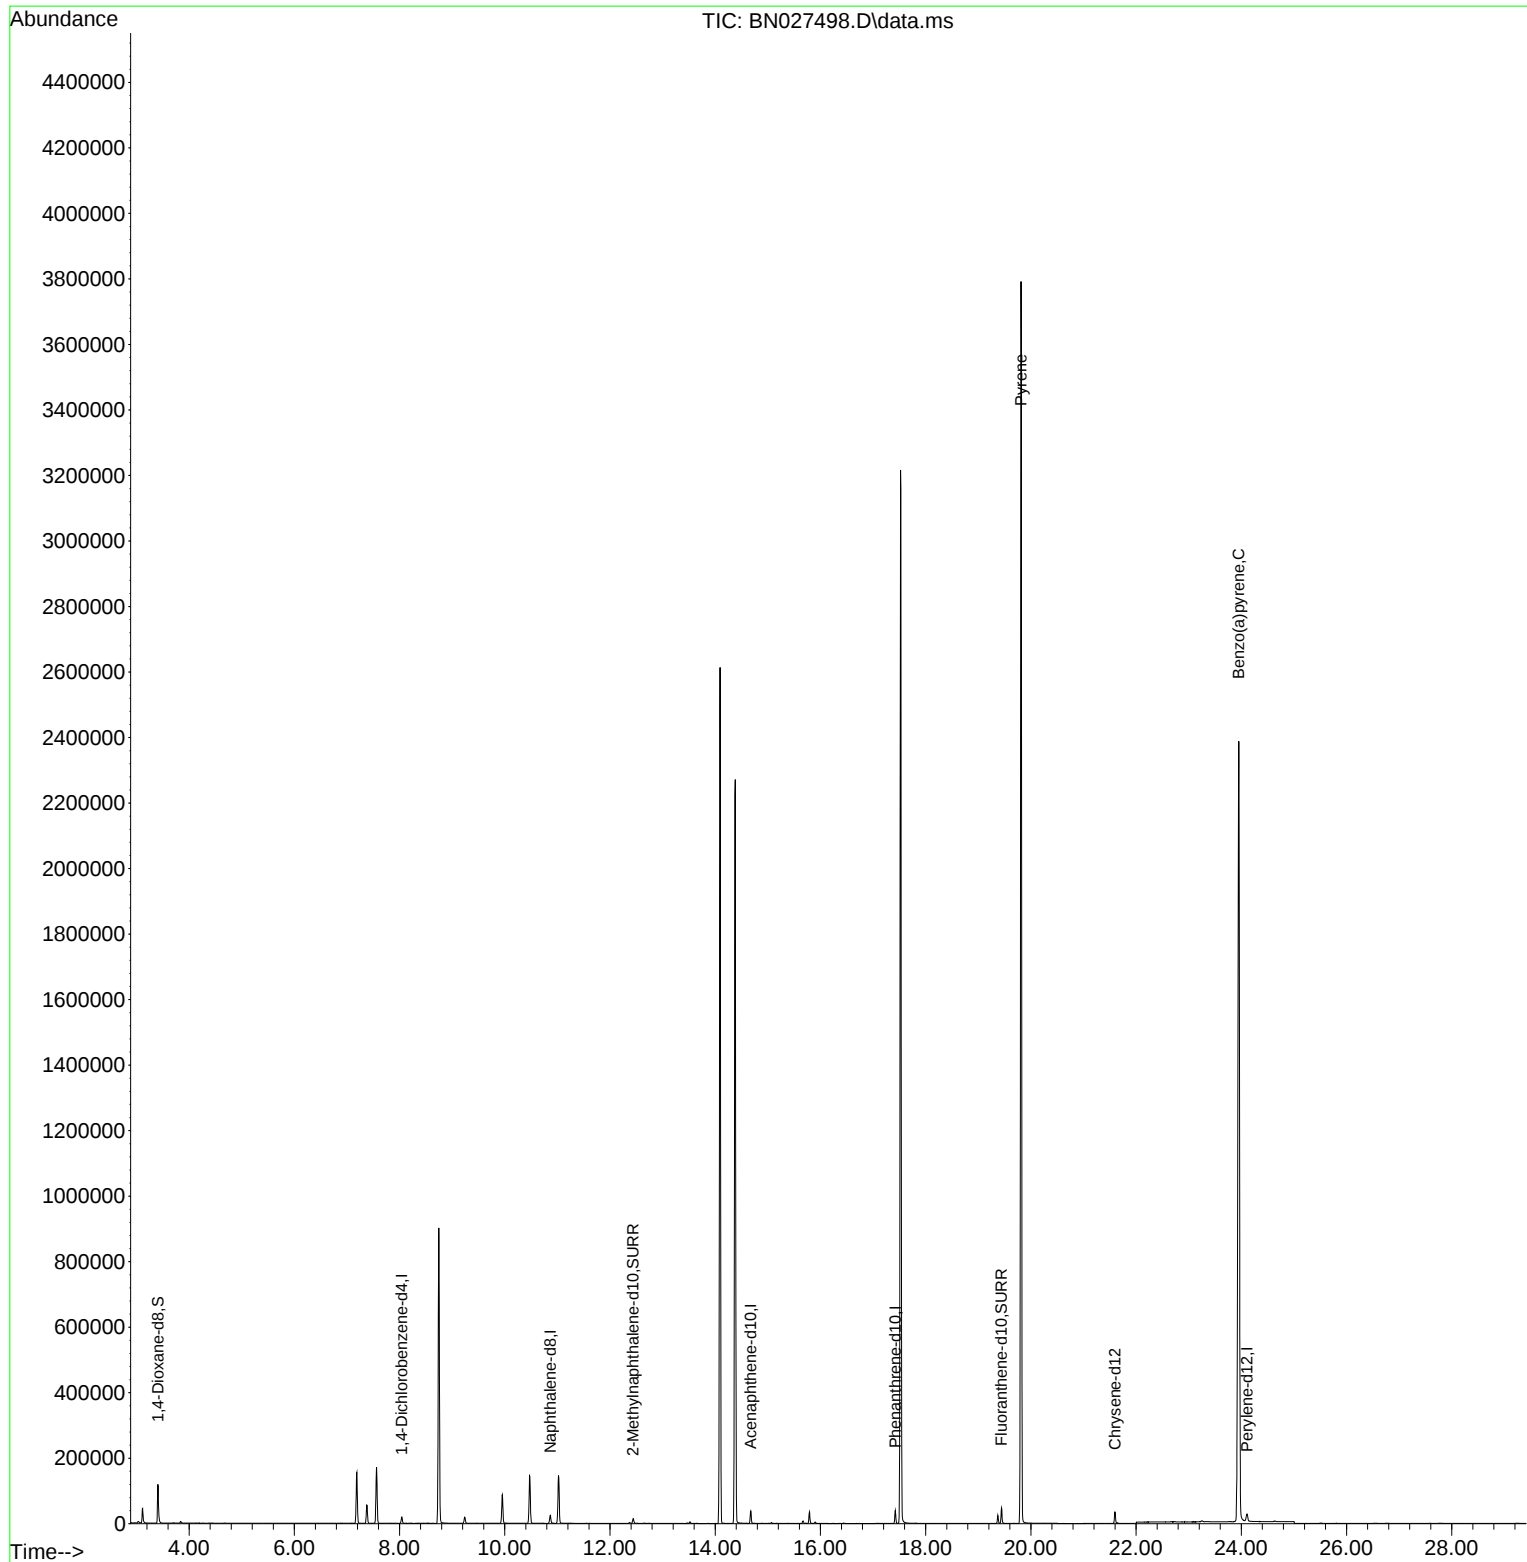

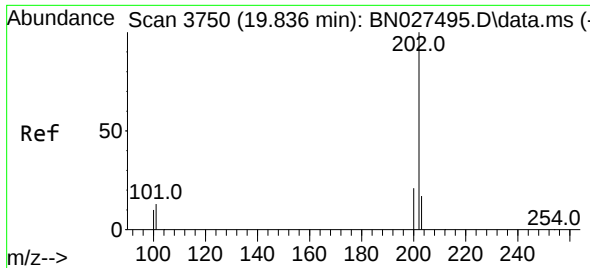

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.813 min Scan# 31

Delta R.T. -0.028 min

Lab File: BN027498.D

Acq: 09 Sep 2023 12:52

Instrument :

BNA_N

ClientSampleId :

SBLK241





Tgt Ion:202 Resp: 6922

Ion Ratio Lower Upper

202 100

101 149.6 11.4 17.2#

100 1111.7 9.4 14.2#

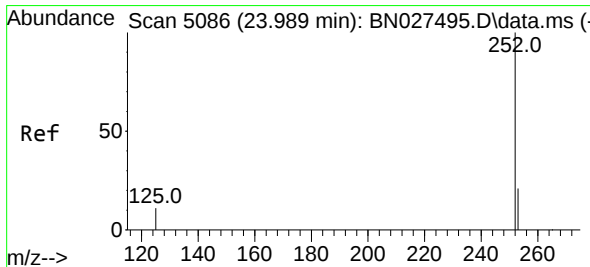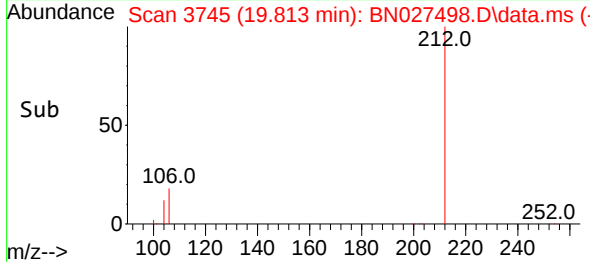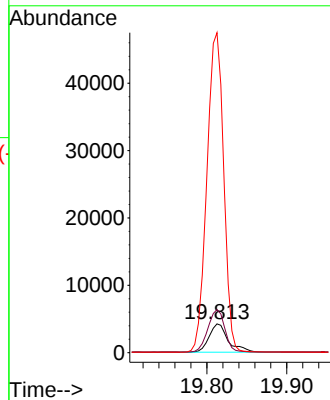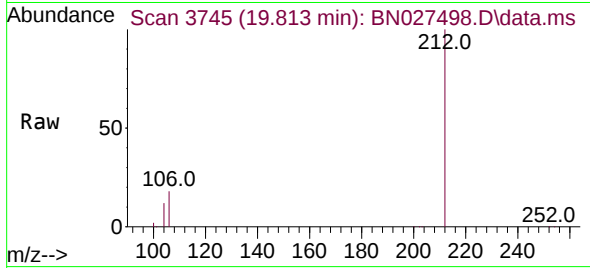

#26

Benzo(a)pyrene

Concen: 0.106 ng/ul

RT: 23.951 min Scan# 5073

Delta R.T. -0.044 min

Lab File: BN027498.D

Acq: 09 Sep 2023 12:52

Tgt Ion:252 Resp: 13384

Ion Ratio Lower Upper

252 100

253 39.2 22.4 33.6#

125 31.0 17.4 26.2#

