

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027512.D
 Acq On : 09 Sep 2023 21:33
 Operator : MA/JU
 Sample : PB155262BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK262

Quant Time: Sep 10 00:54:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	8634	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	29991	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.675	164	18393	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	40587	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	29854	0.400	ng/ul	0.00
23) Perylene-d12	24.103	264	28622	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	65814	5.730	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	16798	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	41882	0.409	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.665	166	5704	0.070	ng/ul#	13
20) Pyrene	19.813	202	5247	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.939	252	9994	0.095	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027512.D
Acq On : 09 Sep 2023 21:33
Operator : MA/JU
Sample : PB155262BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK262

Quant Time: Sep 10 00:54:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




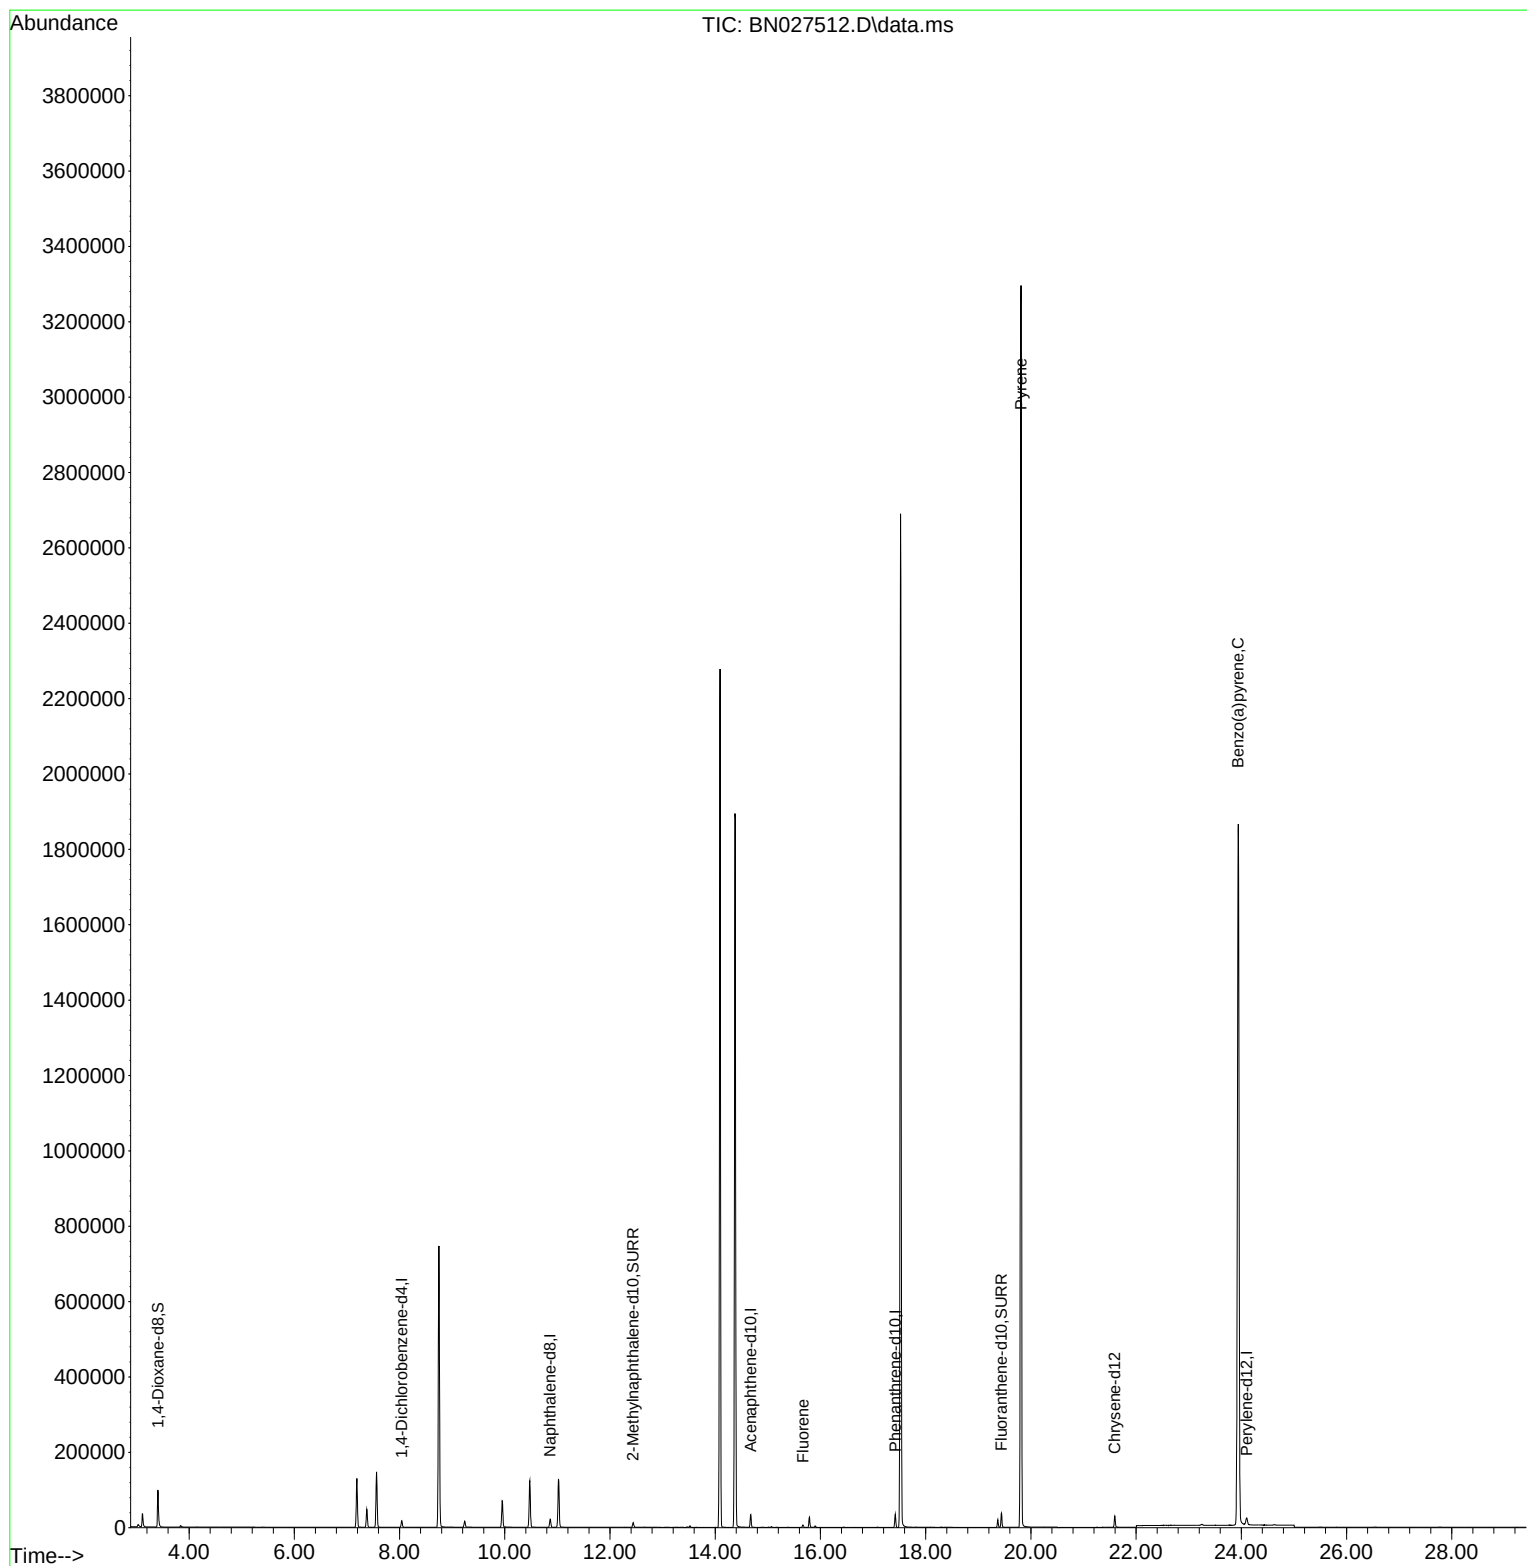


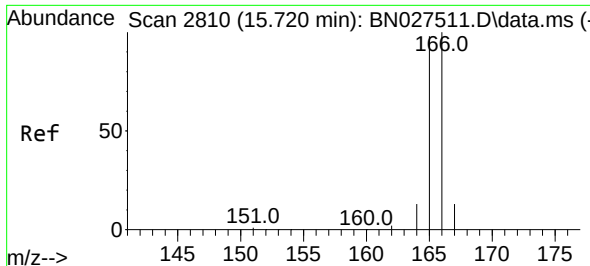

#12
Fluorene
Concen: 0.070 ng/ul
RT: 15.665 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN027512.D
Acq: 09 Sep 2023 21:33




Instrument :
BNA_N
ClientSampleId :
SBLK262


Tgt Ion:166 Resp: 5704
Ion Ratio Lower Upper
166 100
165 6.6 79.6 119.4#
167 32.1 11.4 17.0#

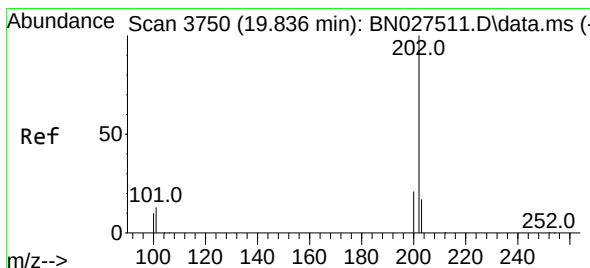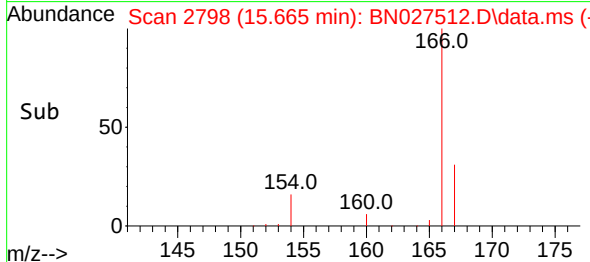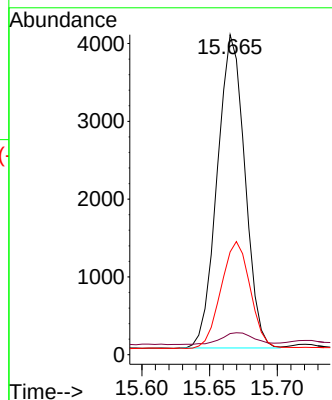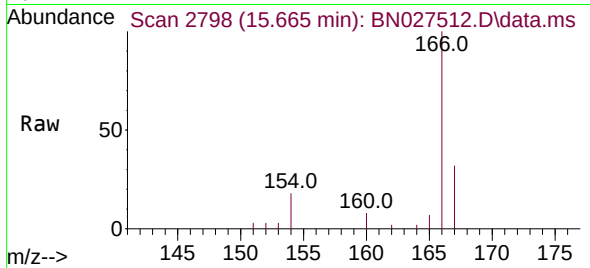

#20
Pyrene
Concen: 0.038 ng/ul
RT: 19.813 min Scan# 3745
Delta R.T. -0.028 min
Lab File: BN027512.D
Acq: 09 Sep 2023 21:33


Tgt Ion:202 Resp: 5247
Ion Ratio Lower Upper
202 100
101 147.8 11.4 17.2#
100 1070.0 9.4 14.2#

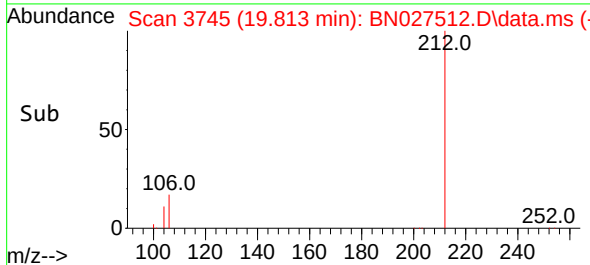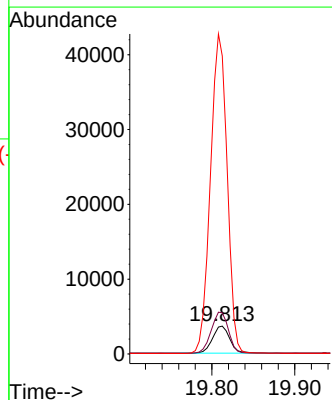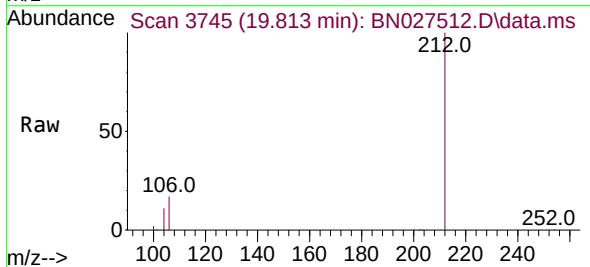

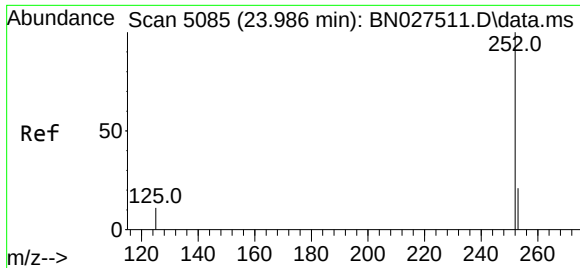

#26
 Benzo(a)pyrene
 Concen: 0.095 ng/ul
 RT: 23.939 min Scan# 50
 Delta R.T. -0.056 min
 Lab File: BN027512.D
 Acq: 09 Sep 2023 21:33

Instrument :
 BNA_N
 ClientSampleId :
 SBLK262

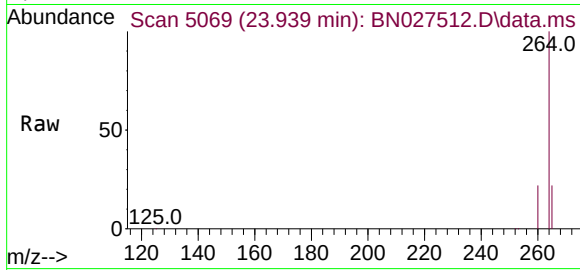

Tgt Ion:252 Resp: 9994

Ion	Ratio	Lower	Upper
252	100		
253	43.8	22.4	33.6#
125	34.6	17.4	26.2#

