

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027513.D
 Acq On : 09 Sep 2023 22:10
 Operator : MA/JU
 Sample : PB155265BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK265

Quant Time: Sep 10 00:54:30 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	7520	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	26060	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.675	164	15904	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	34865	0.400	ng/ul	0.00
17) Chrysene-d12	21.592	240	25291	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	24040	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	65670	6.565	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	16314	0.412	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	38994	0.450	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.808	202	5530	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.939	252	9461	0.107	ng/ul#	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027513.D
Acq On : 09 Sep 2023 22:10
Operator : MA/JU
Sample : PB155265BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK265

Quant Time: Sep 10 00:54:30 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




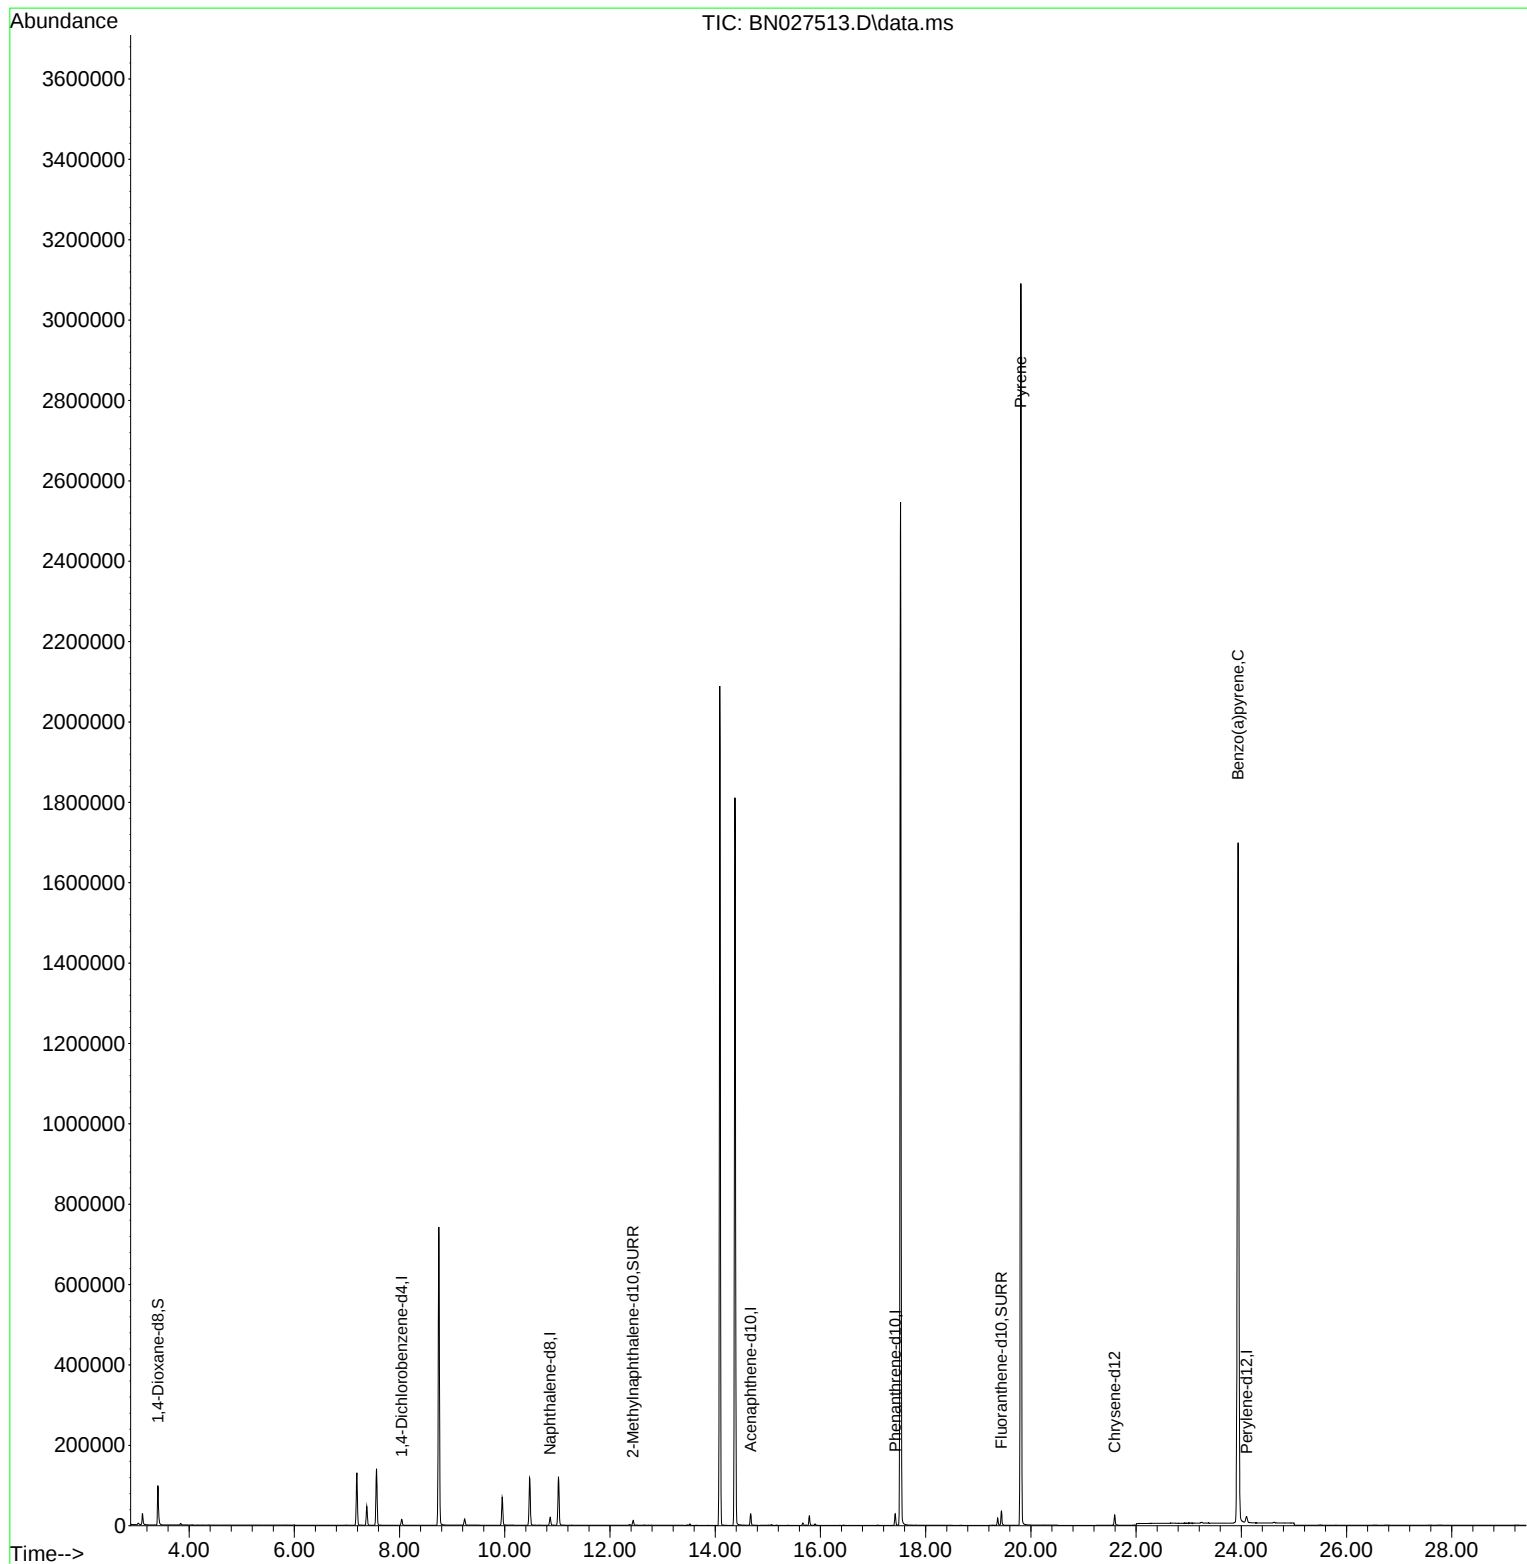


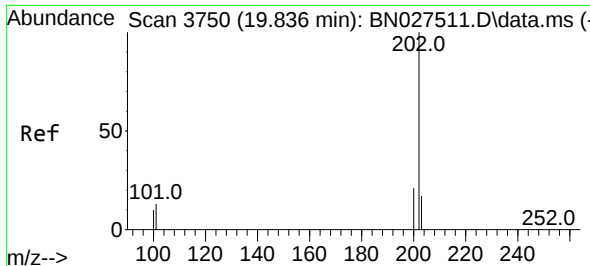

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.808 min Scan# 31
Delta R.T. -0.033 min
Lab File: BN027513.D
Acq: 09 Sep 2023 22:10

Instrument :
BNA_N
ClientSampleId :
SBLK265

Tgt Ion:202 Resp: 5530
Ion Ratio Lower Upper
202 100
101 155.3 11.4 17.2#
100 1181.4 9.4 14.2#

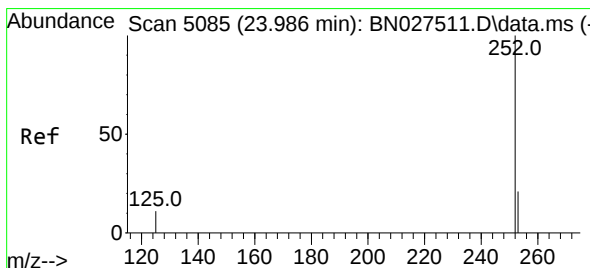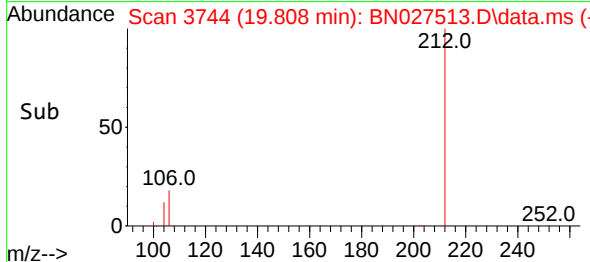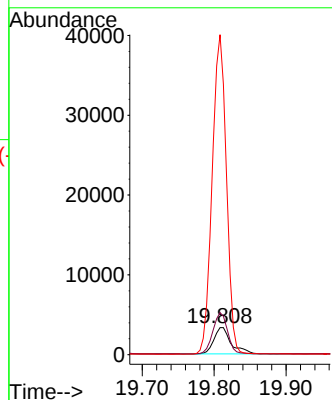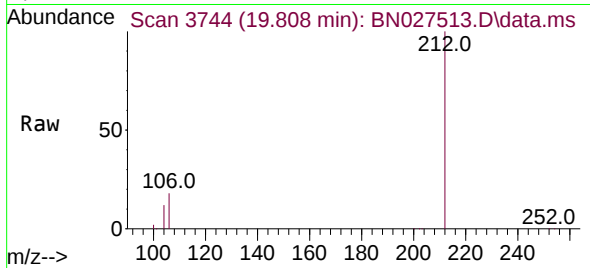

#26
Benzo(a)pyrene
Concen: 0.107 ng/ul
RT: 23.939 min Scan# 5069
Delta R.T. -0.056 min
Lab File: BN027513.D
Acq: 09 Sep 2023 22:10

Tgt Ion:252 Resp: 9461
Ion Ratio Lower Upper
252 100
253 45.8 22.4 33.6#
125 36.5 17.4 26.2#

