

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027534.D
 Acq On : 10 Sep 2023 11:08
 Operator : MA/JU
 Sample : 04250-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4A3

Quant Time: Sep 11 01:18:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	6508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	22539	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164	14158	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.418	188	31274	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	21467	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	20130	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.434	152	12488	0.365	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	30488	0.415	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	1376	0.157	ng/ul#	79
12) Fluorene	15.661	166	4333	0.069	ng/ul#	13
20) Pyrene	19.808	202	3899	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.936	252	7177	0.097	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027534.D
Acq On : 10 Sep 2023 11:08
Operator : MA/JU
Sample : 04250-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH4A3

Quant Time: Sep 11 01:18:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




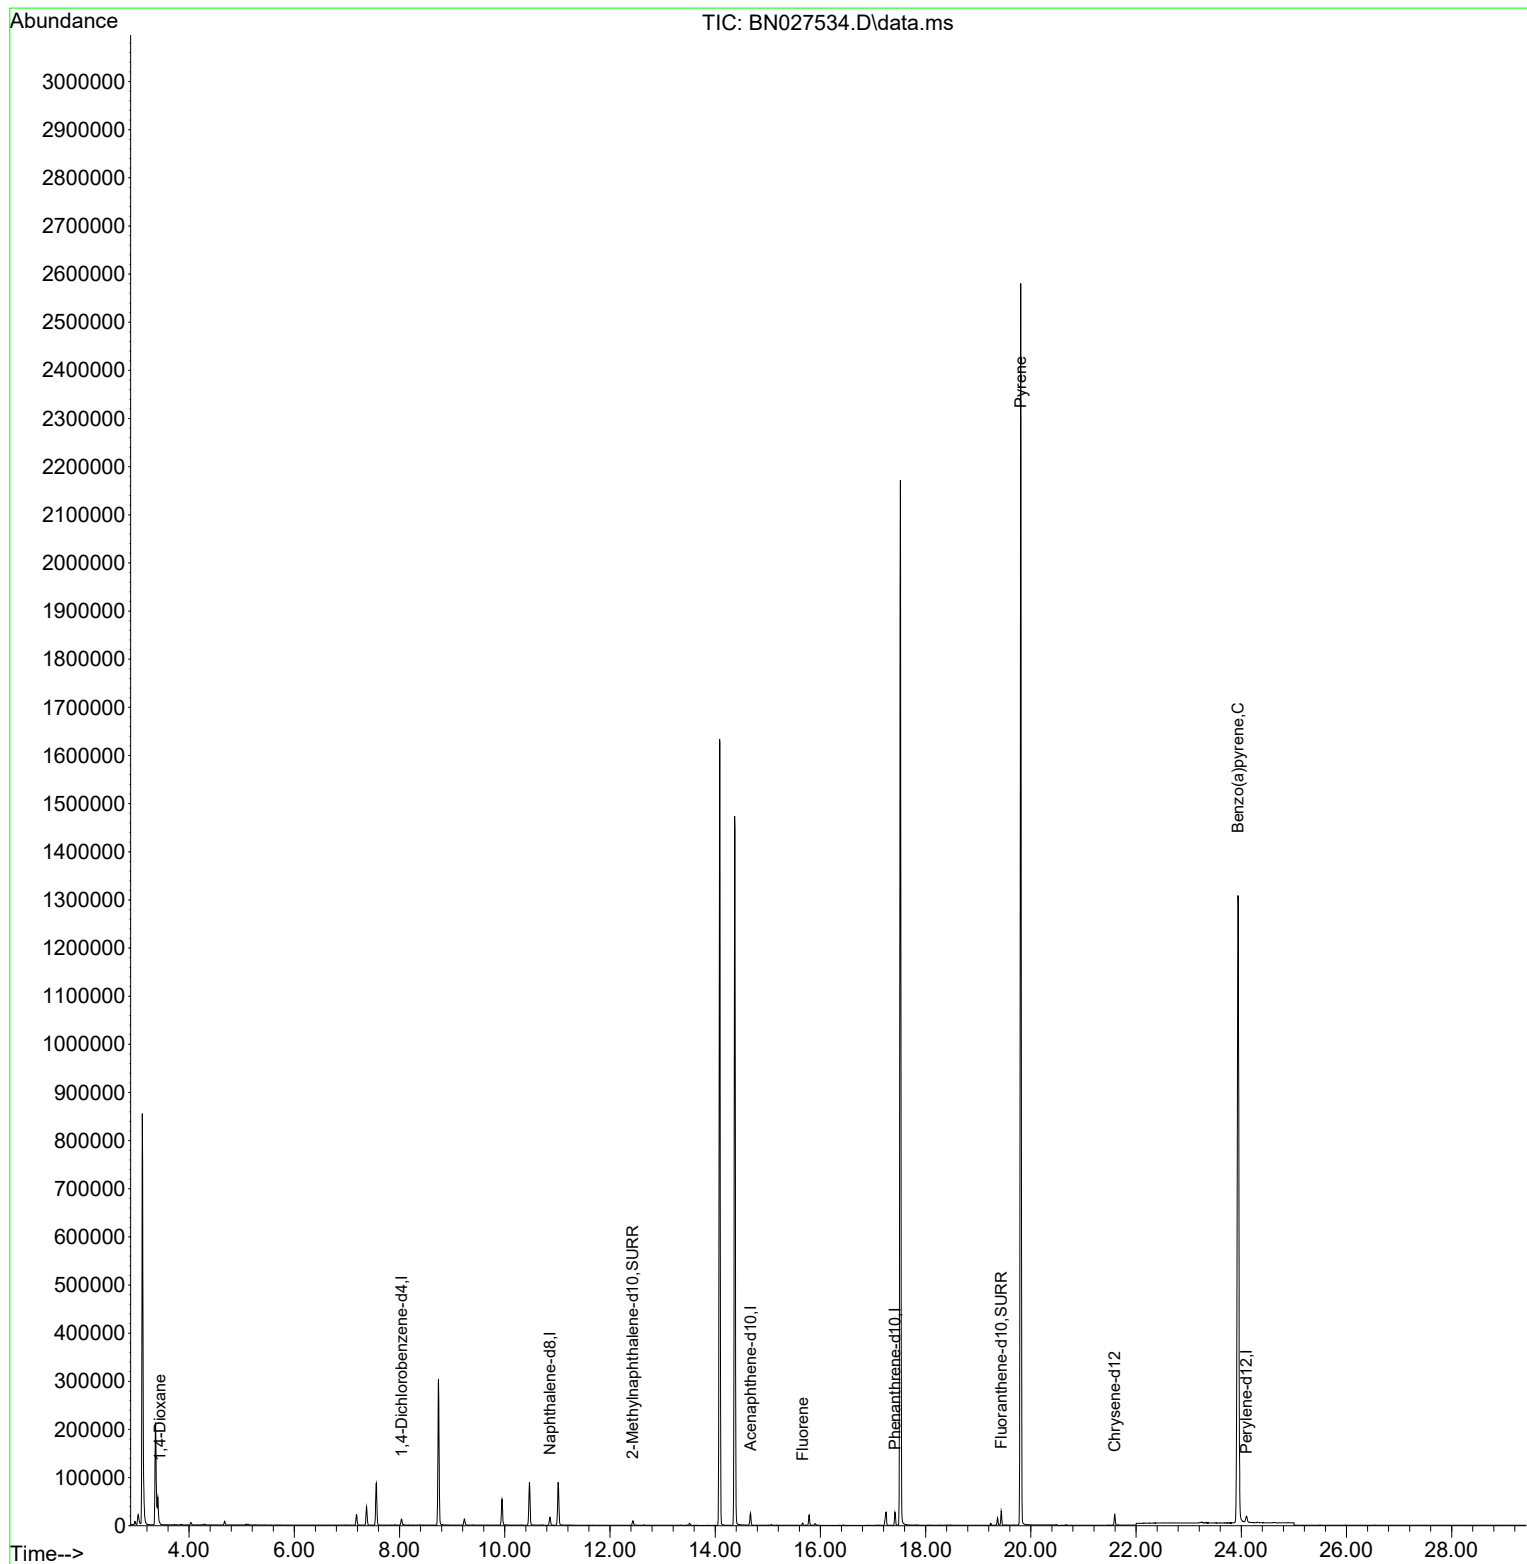


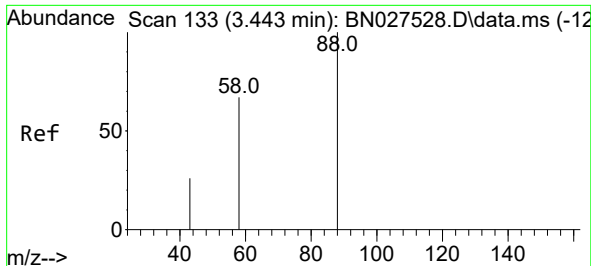

#2
1,4-Dioxane
Concen: 0.157 ng/ul
RT: 3.444 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027534.D
Acq: 10 Sep 2023 11:08




Instrument :
BNA_N
ClientSampleId :
BH4A3


Tgt Ion: 88 Resp: 1376
Ion Ratio Lower Upper
88 100
43 54.6 26.8 40.2#
58 57.1 39.9 59.9

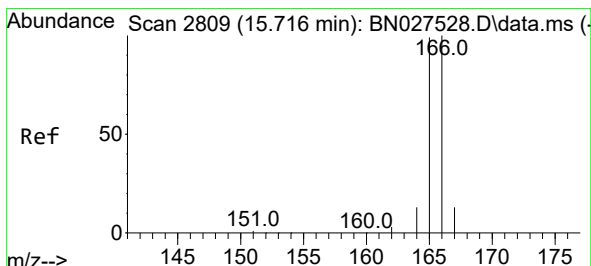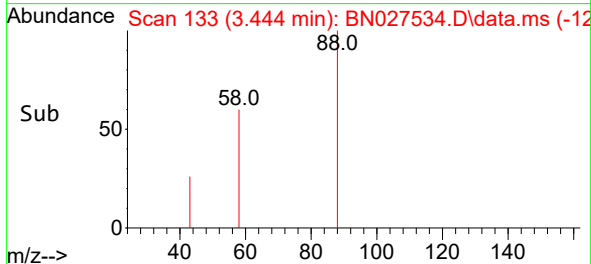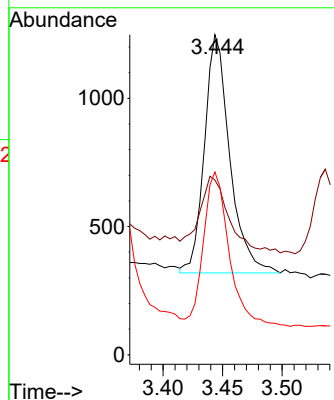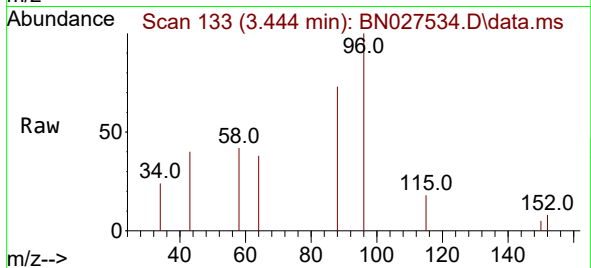

#12
Fluorene
Concen: 0.069 ng/ul
RT: 15.661 min Scan# 2797
Delta R.T. -0.065 min
Lab File: BN027534.D
Acq: 10 Sep 2023 11:08

Tgt Ion:166 Resp: 4333
Ion Ratio Lower Upper
166 100
165 7.5 79.6 119.4#
167 33.7 11.4 17.0#

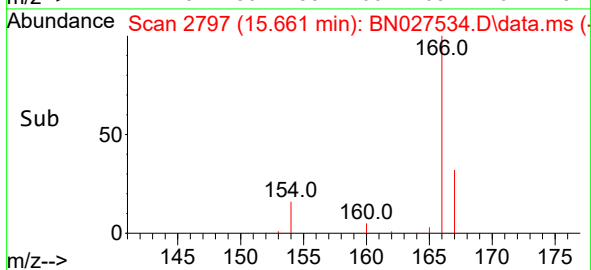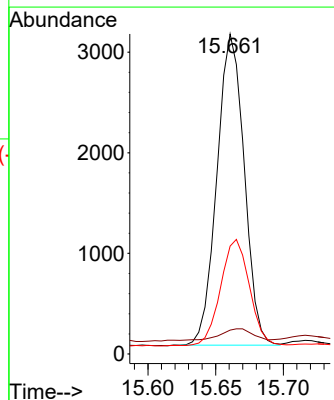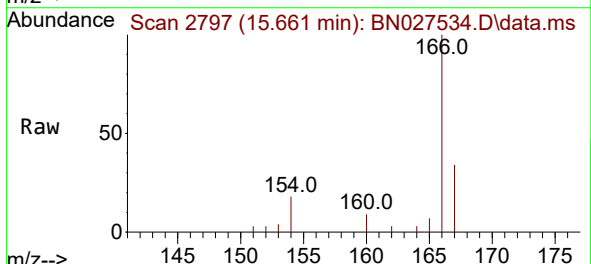

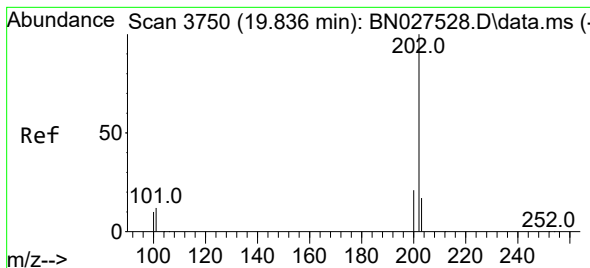

#20

Pyrene

Concen: 0.039 ng/ul

RT: 19.808 min Scan# 31

Delta R.T. -0.033 min

Lab File: BN027534.D

Acq: 10 Sep 2023 11:08

Instrument :

BNA_N

ClientSampleId :

BH4A3





Tgt Ion:202 Resp: 3899

Ion Ratio Lower Upper

202 100

101 150.3 11.4 17.2#

100 1107.4 9.4 14.2#

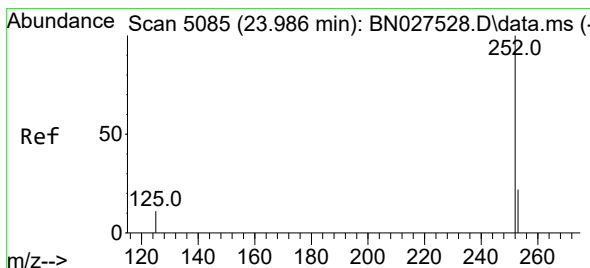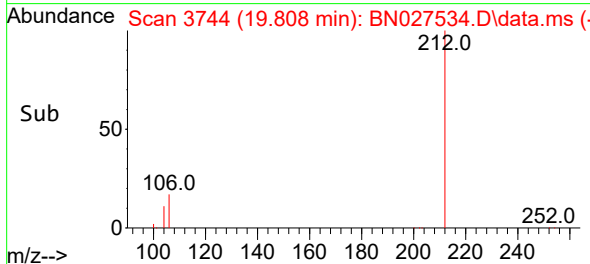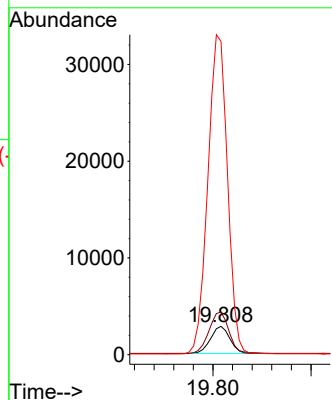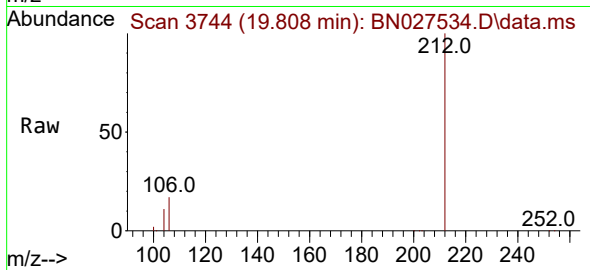

#26

Benzo(a)pyrene

Concen: 0.097 ng/ul

RT: 23.936 min Scan# 5068

Delta R.T. -0.058 min

Lab File: BN027534.D

Acq: 10 Sep 2023 11:08

Tgt Ion:252 Resp: 7177

Ion Ratio Lower Upper

252 100

253 47.3 22.4 33.6#

125 40.6 17.4 26.2#

