

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027537.D
 Acq On : 10 Sep 2023 12:57
 Operator : MA/JU
 Sample : 04268-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0GH2

Quant Time: Sep 11 01:19:00 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	5751	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	19759	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	12038	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.417	188	25980	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	17830	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	16364	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	27483	3.593	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	9768	0.326	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	26369	0.432	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.808	202	3527	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.936	252	6019	0.100	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027537.D
Acq On : 10 Sep 2023 12:57
Operator : MA/JU
Sample : 04268-02
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0GH2

Quant Time: Sep 11 01:19:00 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




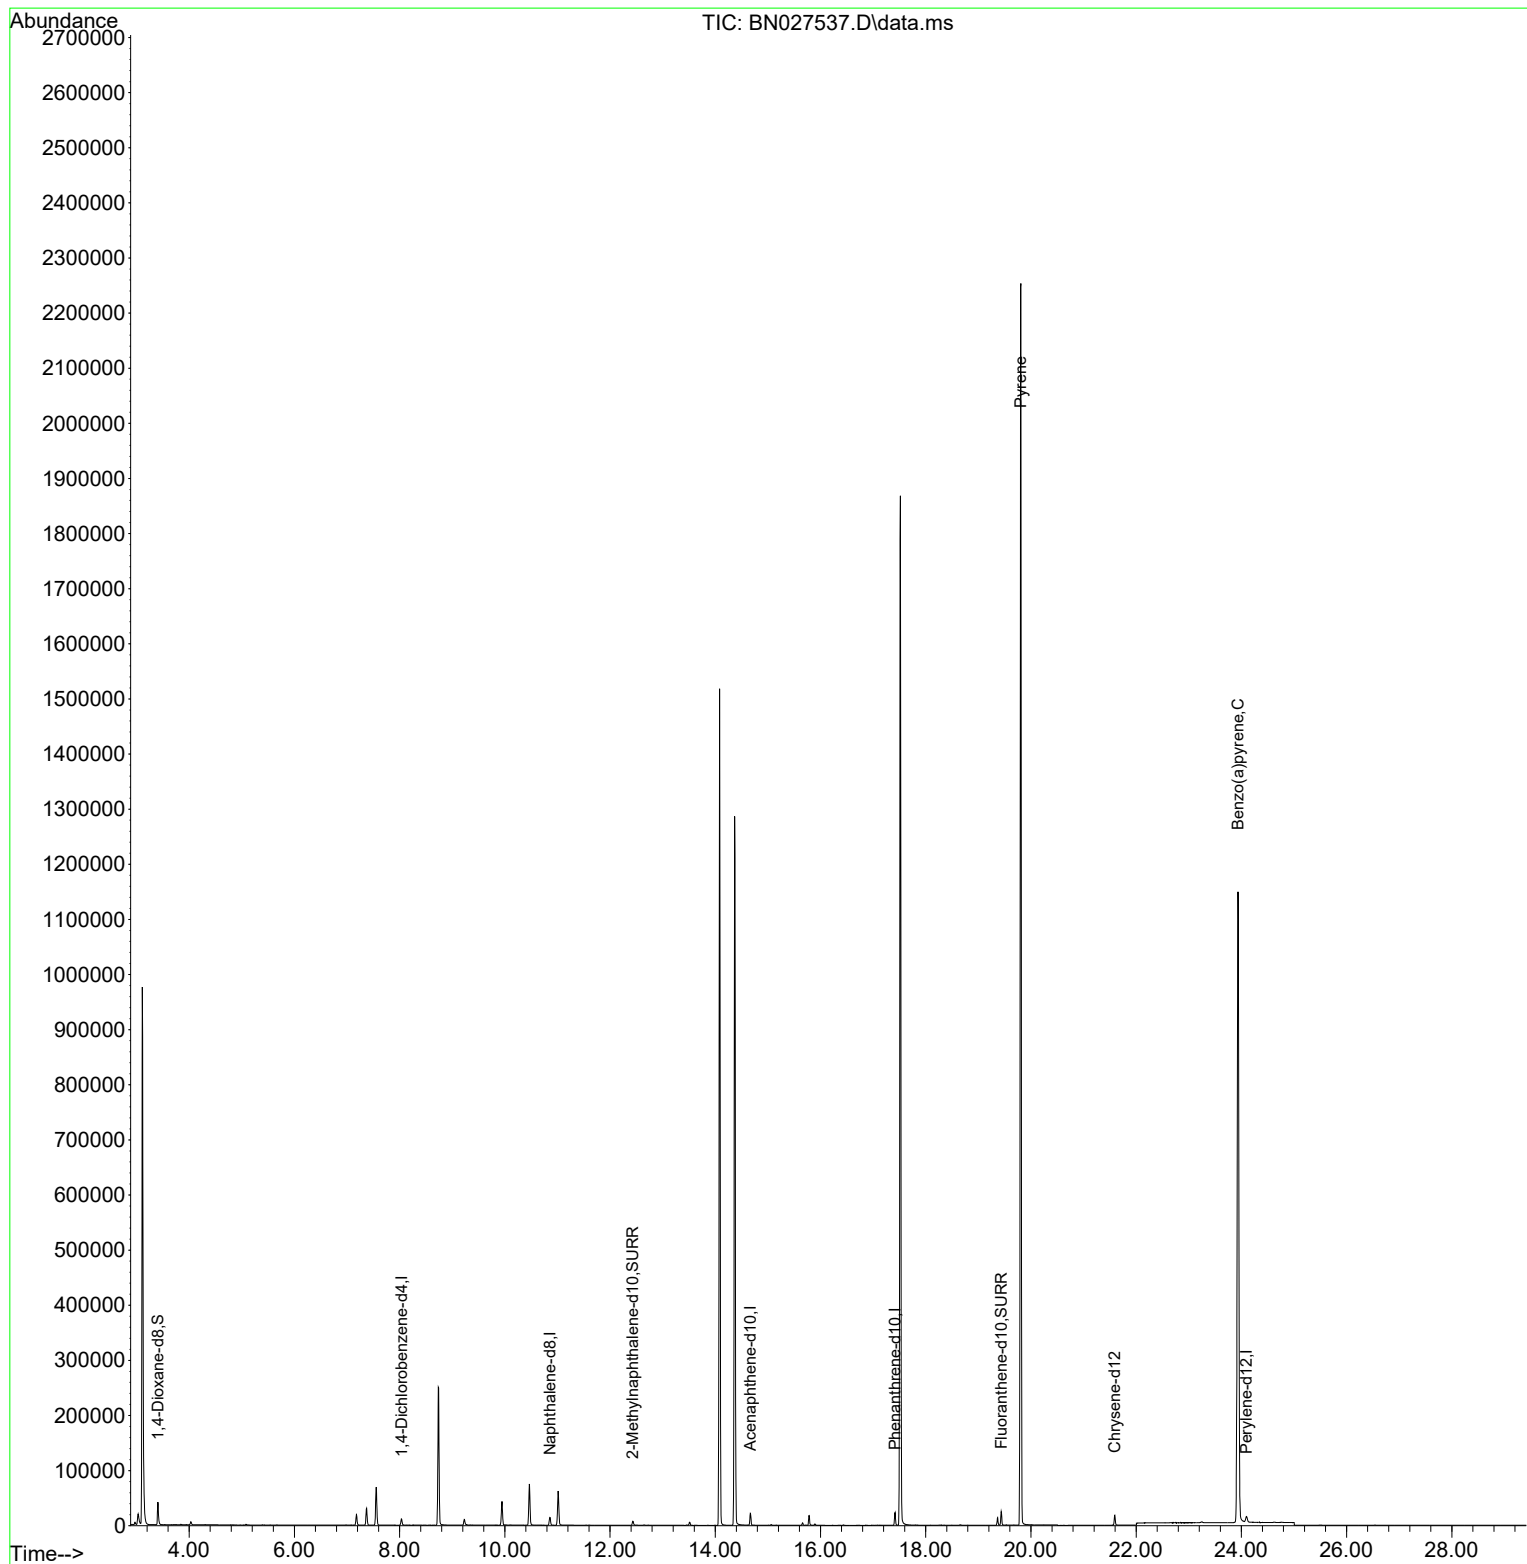


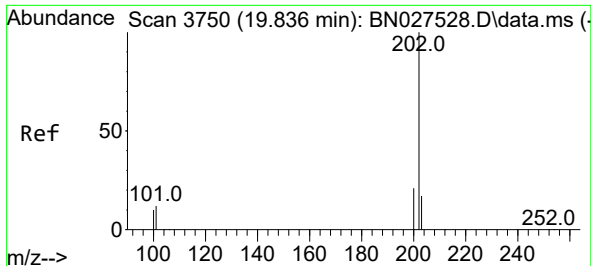

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.808 min Scan# 31
Delta R.T. -0.033 min
Lab File: BN027537.D
Acq: 10 Sep 2023 12:57

Instrument :
BNA_N
ClientSampleId :
H0GH2

Tgt Ion:202 Resp: 3527
Ion Ratio Lower Upper
202 100
101 151.3 11.4 17.2#
100 1111.1 9.4 14.2#

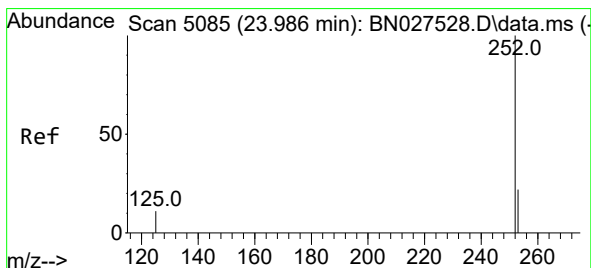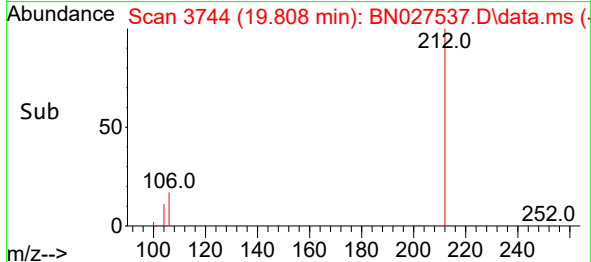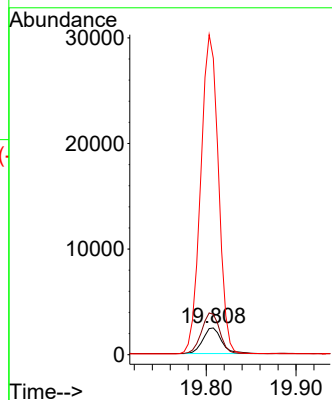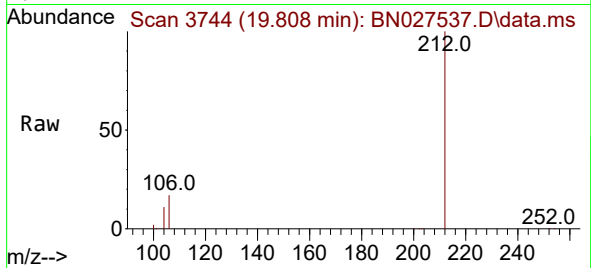

#26
Benzo(a)pyrene
Concen: 0.100 ng/ul
RT: 23.936 min Scan# 5068
Delta R.T. -0.059 min
Lab File: BN027537.D
Acq: 10 Sep 2023 12:57

Tgt Ion:252 Resp: 6019
Ion Ratio Lower Upper
252 100
253 48.3 22.4 33.6#
125 42.0 17.4 26.2#

