

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027544.D
 Acq On : 10 Sep 2023 17:15
 Operator : MA/JU
 Sample : PB155341BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK341

Quant Time: Sep 11 01:20:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	7408	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	25509	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.670	164	15175	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	32361	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	20961	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	18620	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	53198	5.398	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	12214	0.315	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	25388	0.353	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.660	166	4303	0.064	ng/ul#	13
20) Pyrene	19.808	202	3583	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.933	252	5940	0.086	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027544.D
Acq On : 10 Sep 2023 17:15
Operator : MA/JU
Sample : PB155341BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK341

Quant Time: Sep 11 01:20:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




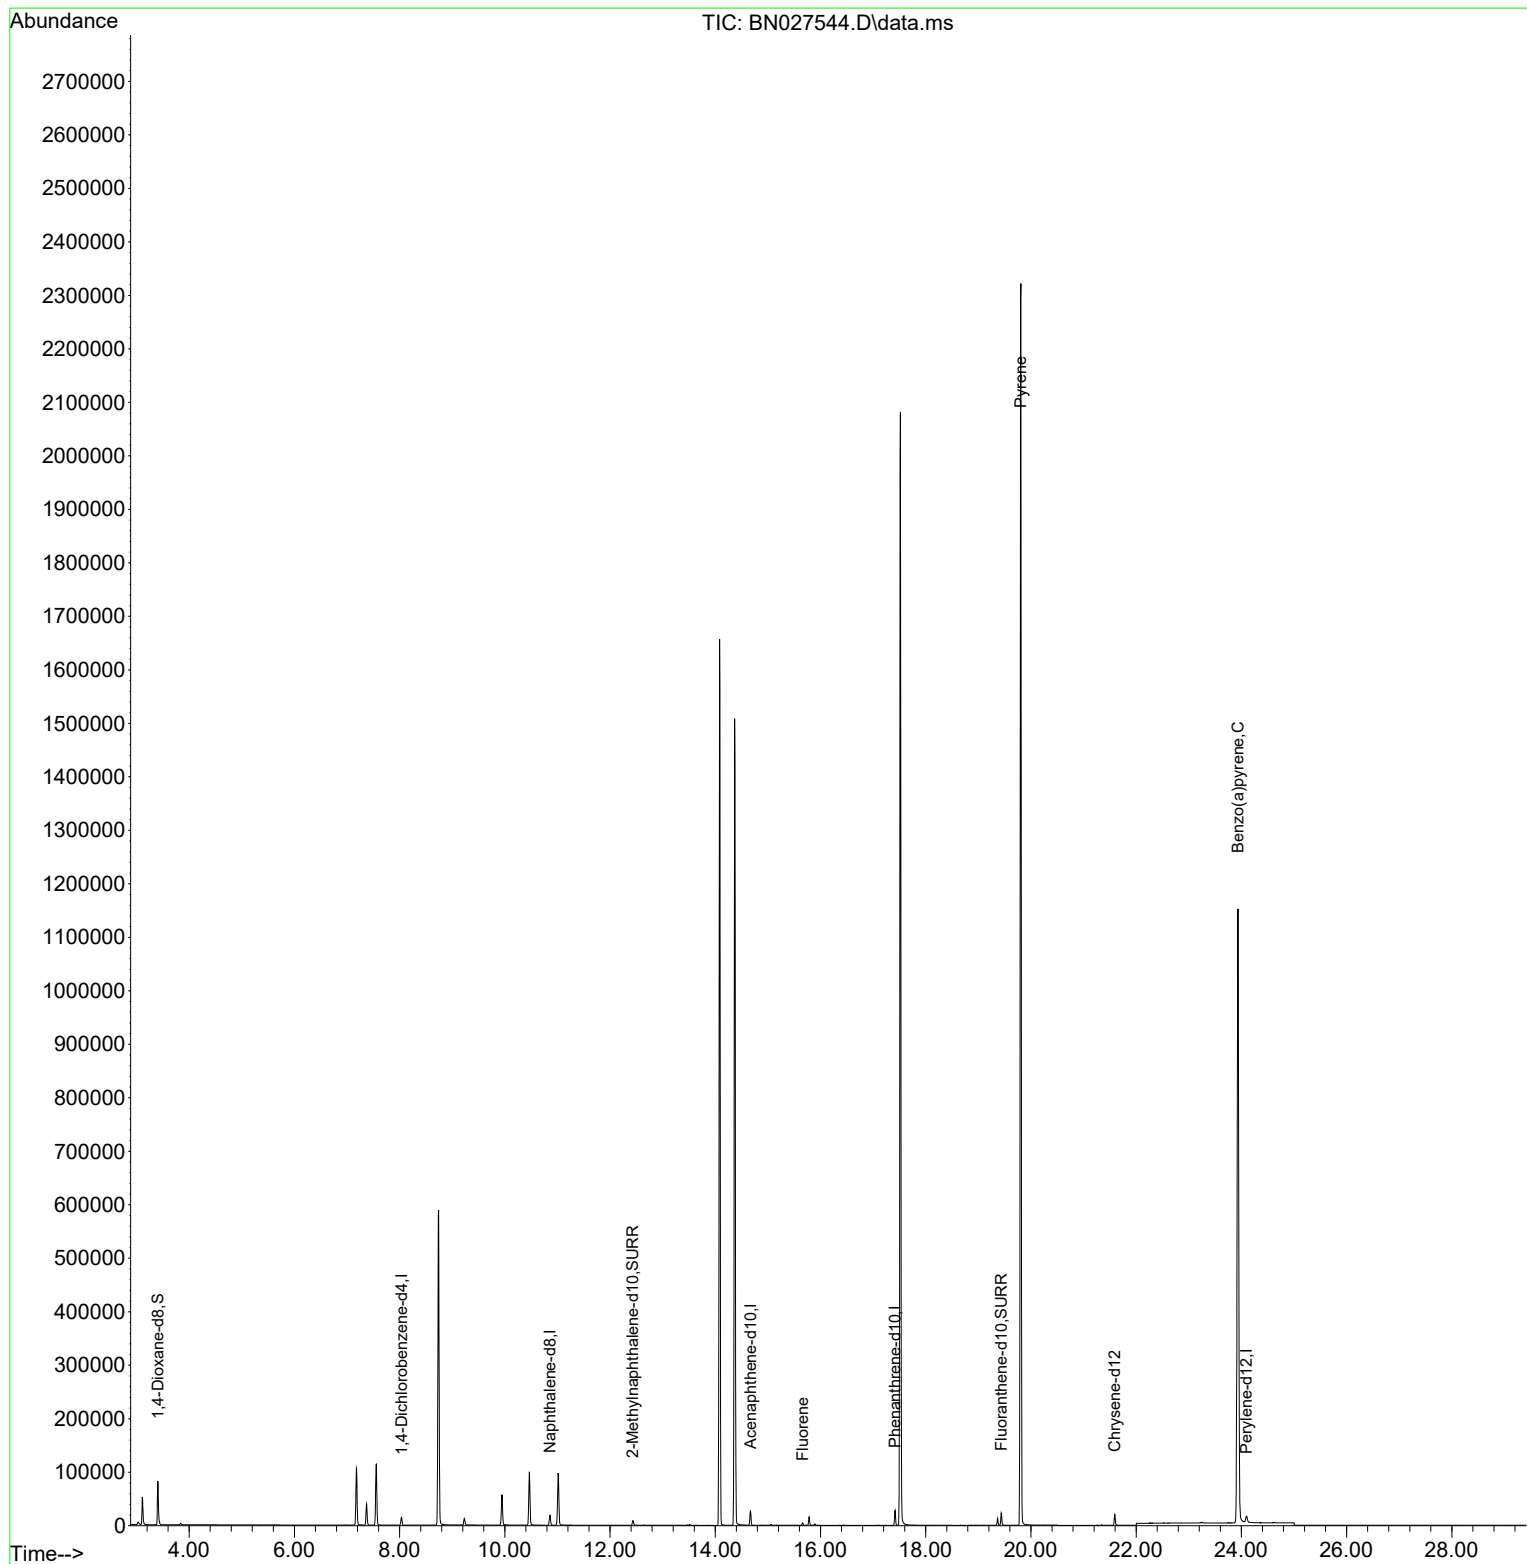


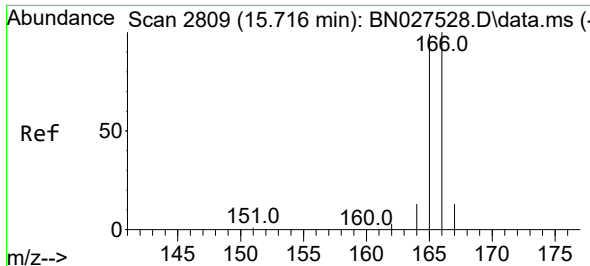

#12
Fluorene
Concen: 0.064 ng/ul
RT: 15.660 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN027544.D
Acq: 10 Sep 2023 17:15




Instrument :
BNA_N
ClientSampleId :
SBLK341


Tgt Ion:166 Resp: 4303
Ion Ratio Lower Upper
166 100
165 6.9 79.6 119.4#
167 32.8 11.4 17.0#

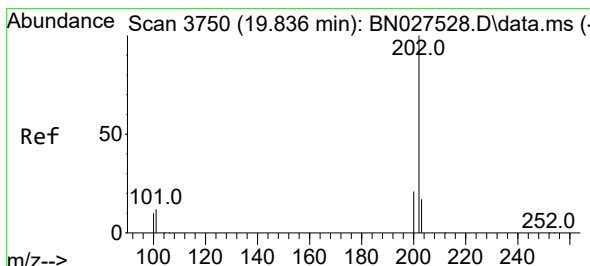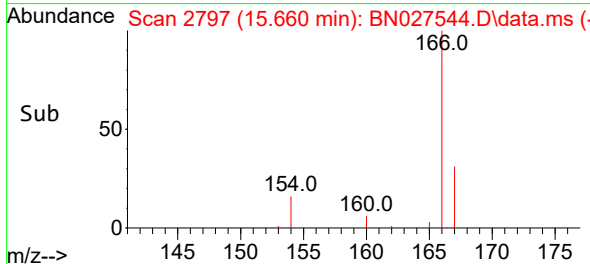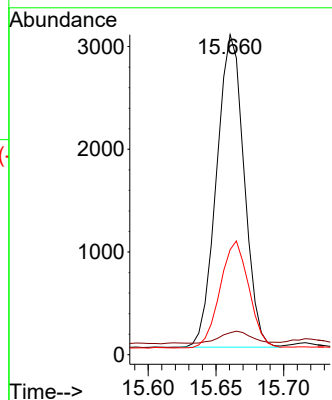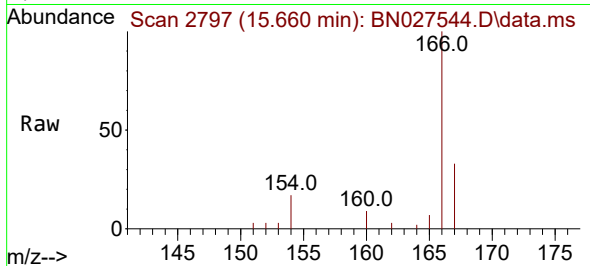

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.808 min Scan# 3744
Delta R.T. -0.033 min
Lab File: BN027544.D
Acq: 10 Sep 2023 17:15


Tgt Ion:202 Resp: 3583
Ion Ratio Lower Upper
202 100
101 151.0 11.4 17.2#
100 1093.2 9.4 14.2#

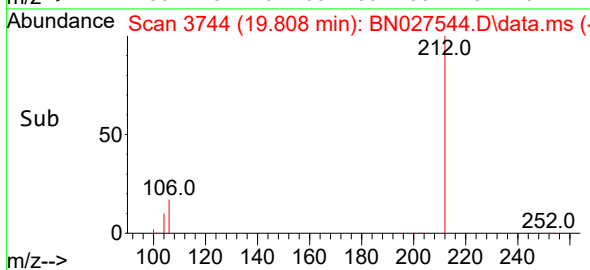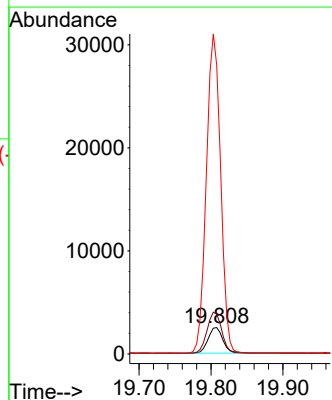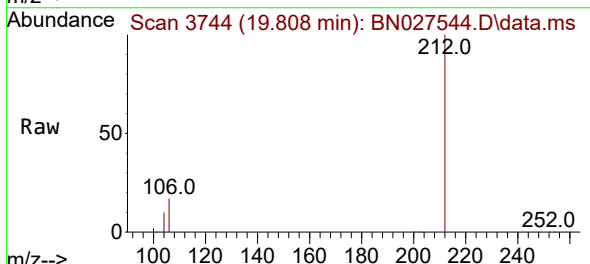

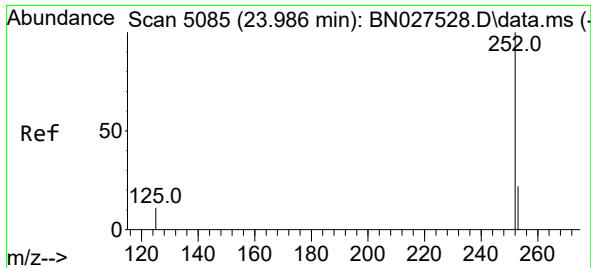

#26
Benzo(a)pyrene
Concen: 0.086 ng/ul
RT: 23.933 min Scan# 50
Delta R.T. -0.062 min
Lab File: BN027544.D
Acq: 10 Sep 2023 17:15

Instrument :
BNA_N
ClientSampleId :
SBLK341

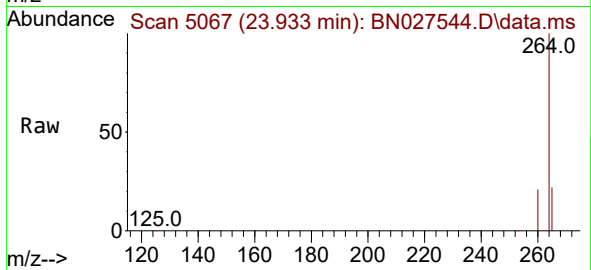

Tgt Ion:252 Resp: 5940
Ion Ratio Lower Upper
252 100
253 46.0 22.4 33.6#
125 40.2 17.4 26.2#

