

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027545.D
 Acq On : 10 Sep 2023 17:52
 Operator : MA/JU
 Sample : PB155344BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK344

Quant Time: Sep 11 01:20:23 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	6890	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	23583	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.670	164	14143	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188	30202	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	19231	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	17437	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	49479	5.399	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	11266	0.315	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	23542	0.357	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.660	166	3991	0.064	ng/ul#	13
20) Pyrene	19.803	202	3352	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.936	252	5468	0.085	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027545.D
Acq On : 10 Sep 2023 17:52
Operator : MA/JU
Sample : PB155344BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK344

Quant Time: Sep 11 01:20:23 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




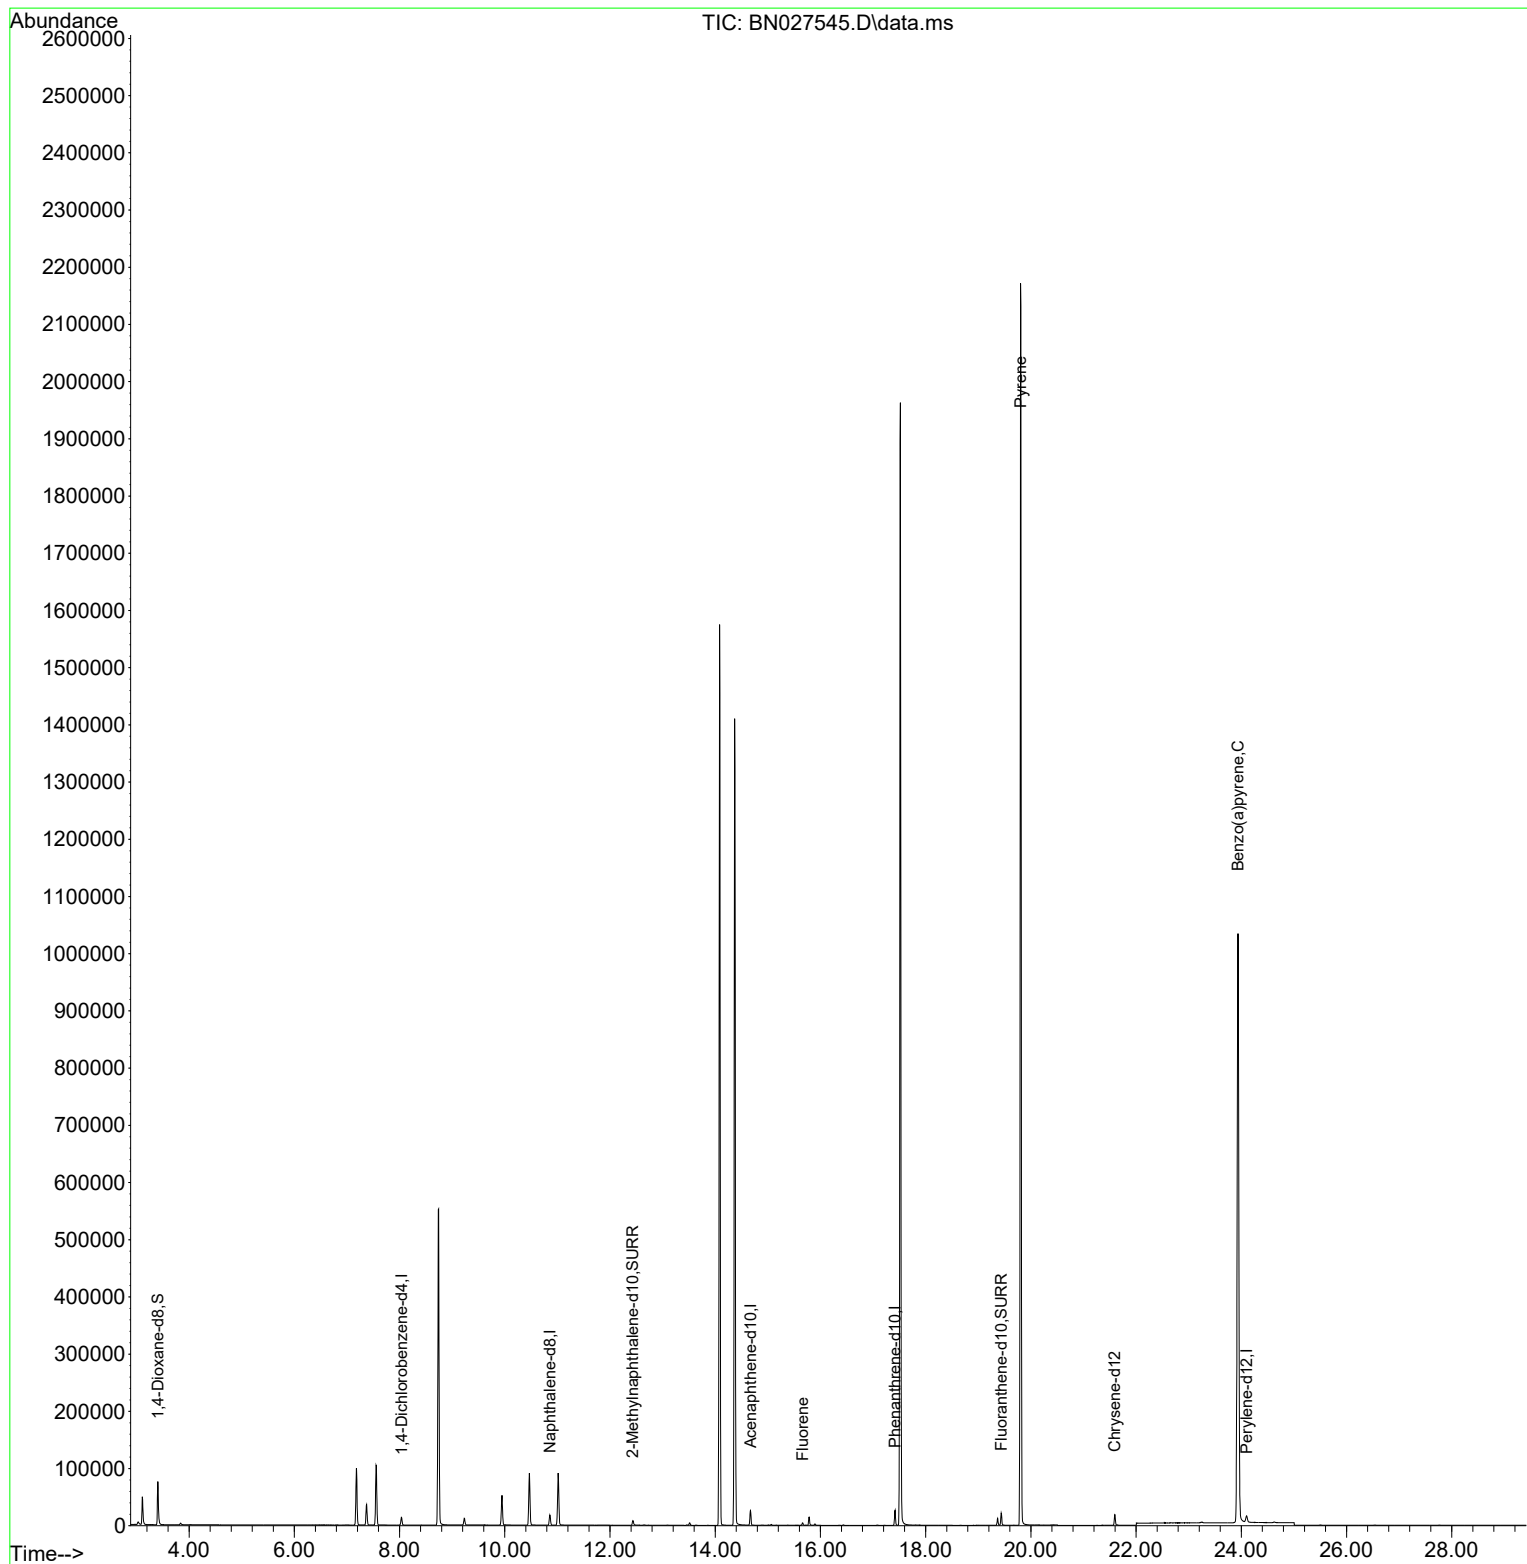


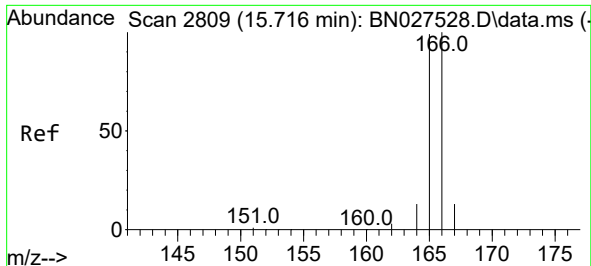

#12
Fluorene
Concen: 0.064 ng/ul
RT: 15.660 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN027545.D
Acq: 10 Sep 2023 17:52




Instrument :
BNA_N
ClientSampleId :
SBLK344


Tgt Ion:166 Resp: 3991
Ion Ratio Lower Upper
166 100
165 7.2 79.6 119.4#
167 34.0 11.4 17.0#

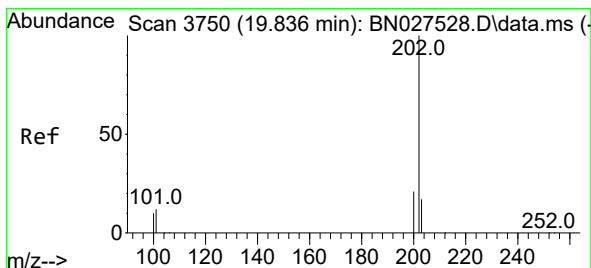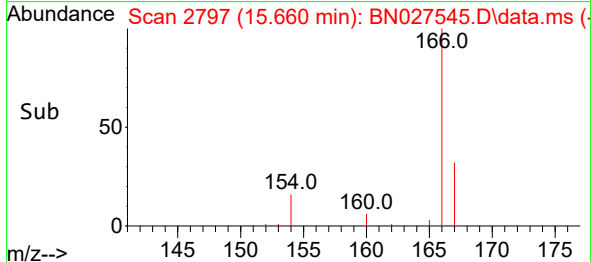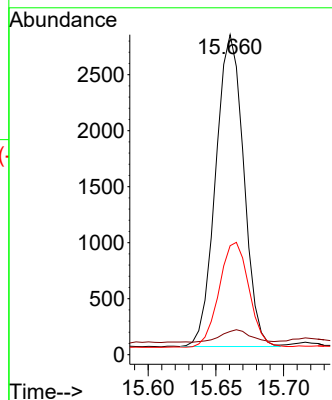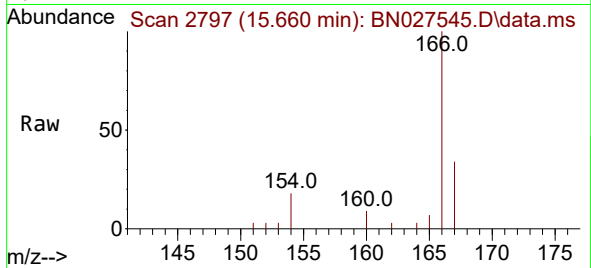

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.803 min Scan# 3743
Delta R.T. -0.037 min
Lab File: BN027545.D
Acq: 10 Sep 2023 17:52


Tgt Ion:202 Resp: 3352
Ion Ratio Lower Upper
202 100
101 160.0 11.4 17.2#
100 1217.6 9.4 14.2#

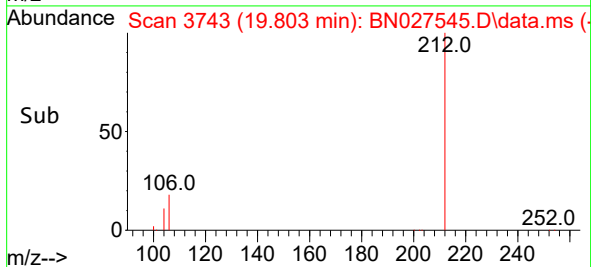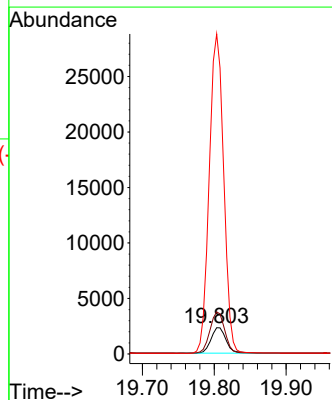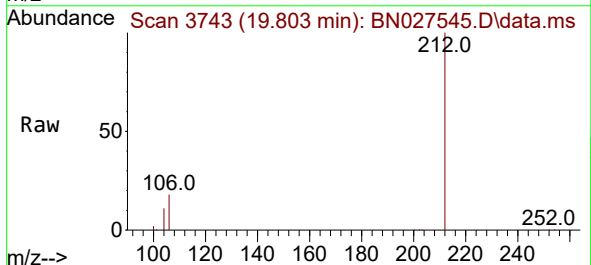

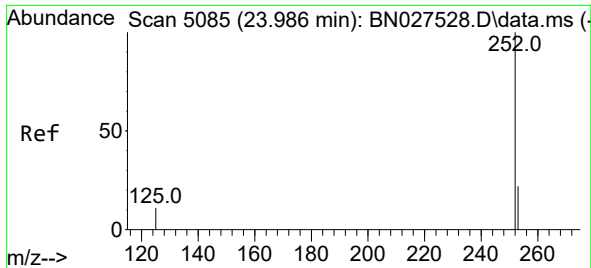

#26
Benzo(a)pyrene
Concen: 0.085 ng/ul
RT: 23.936 min Scan# 50
Delta R.T. -0.059 min
Lab File: BN027545.D
Acq: 10 Sep 2023 17:52

Instrument :
BNA_N
ClientSampleId :
SBLK344

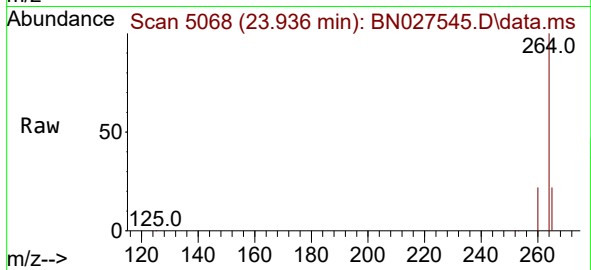

Tgt Ion:252 Resp: 5468
Ion Ratio Lower Upper
252 100
253 48.8 22.4 33.6#
125 42.7 17.4 26.2#

