

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027546.D
 Acq On : 10 Sep 2023 18:29
 Operator : MA/JU
 Sample : PB155348BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK348

Quant Time: Sep 11 01:20:29 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	6729	0.400	ng/ul	0.00
4) Naphthalene-d8	10.856	136	23050	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	14049	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.417	188	29905	0.400	ng/ul	0.00
17) Chrysene-d12	21.592	240	19013	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	16055	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	37965	4.241	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	8536	0.244	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	18847	0.289	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.660	166	3095	0.050	ng/ul#	14
20) Pyrene	19.808	202	2664	0.030	ng/ul#	1
26) Benzo(a)pyrene	23.933	252	4284	0.072	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027546.D
Acq On : 10 Sep 2023 18:29
Operator : MA/JU
Sample : PB155348BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK348

Quant Time: Sep 11 01:20:29 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




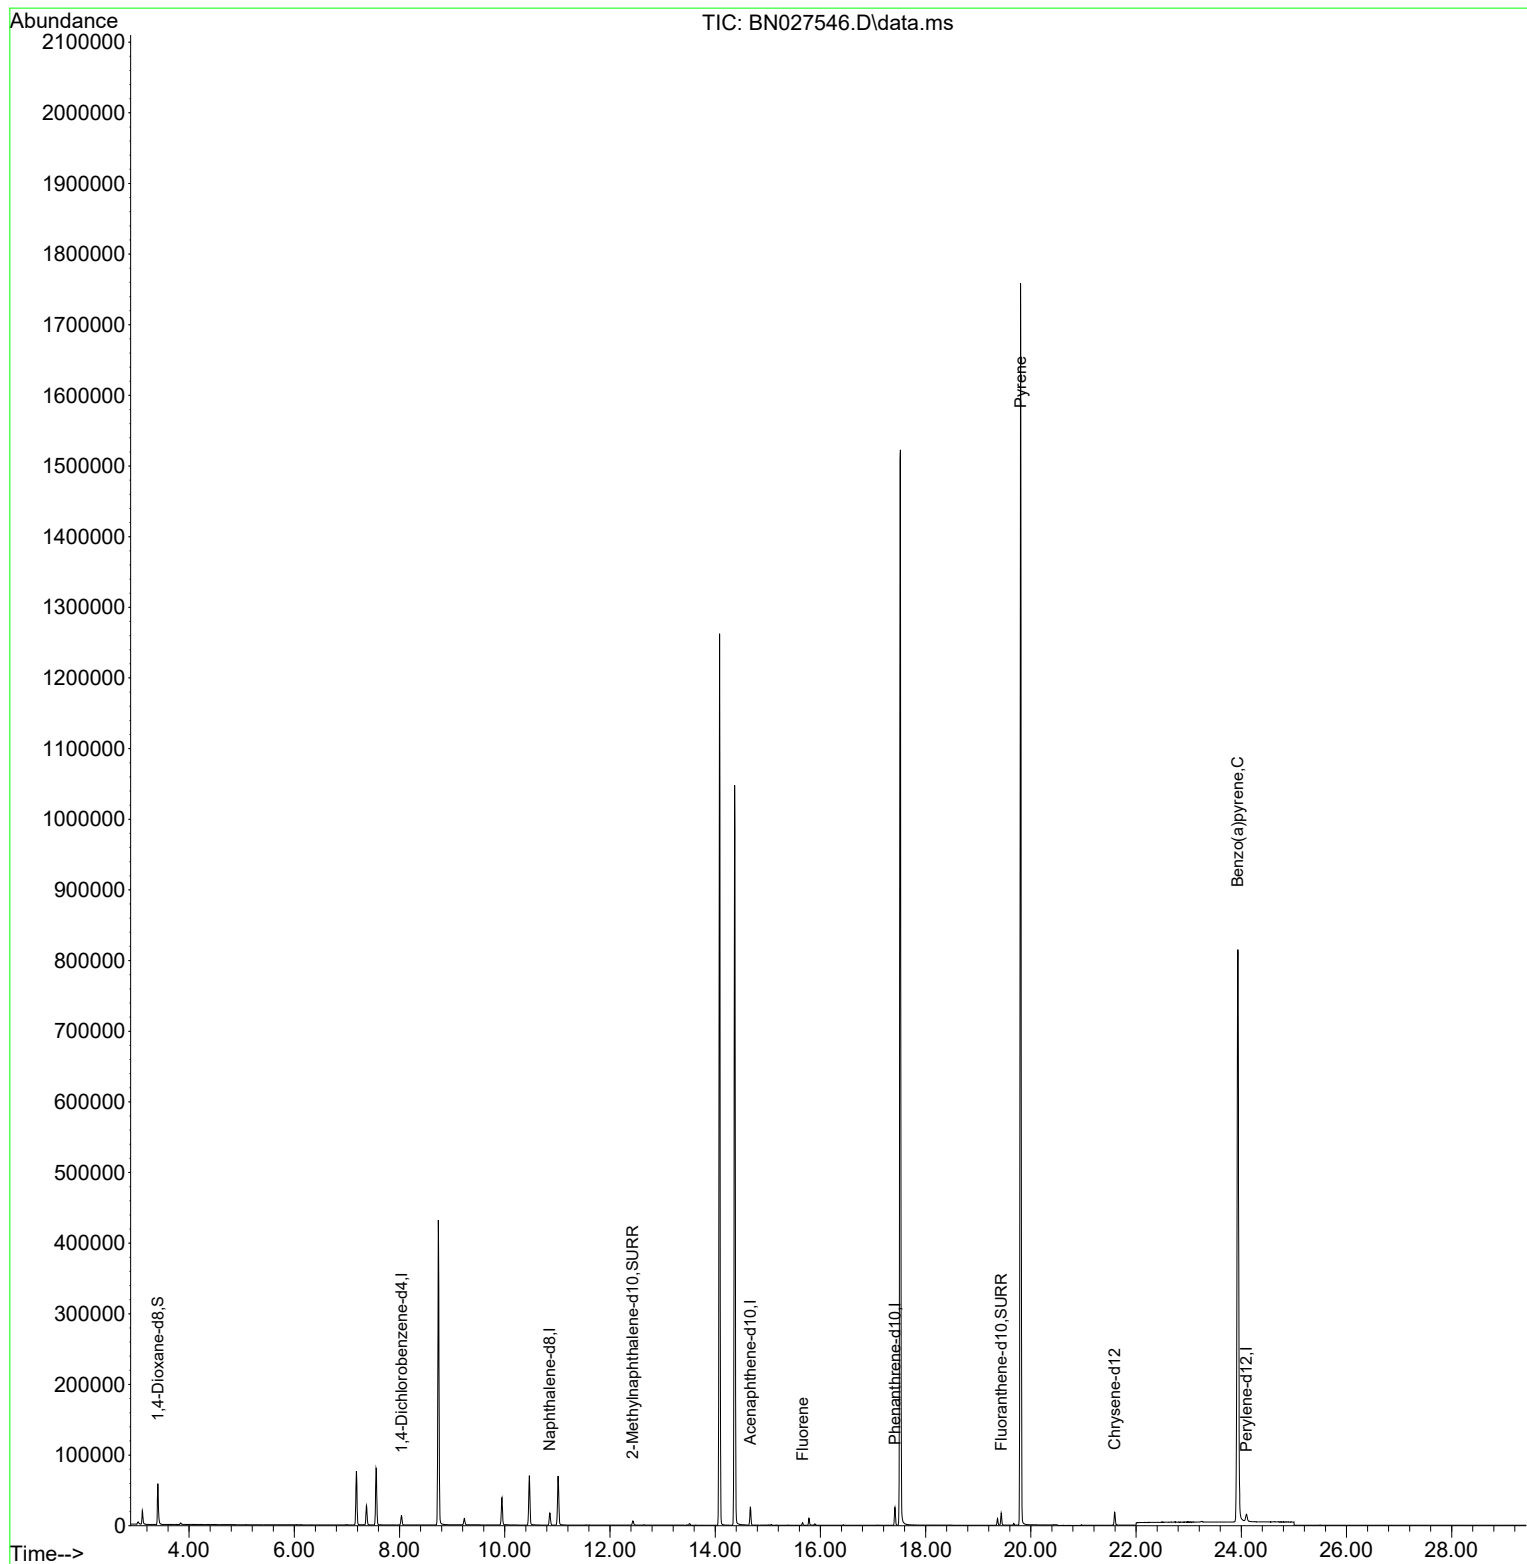


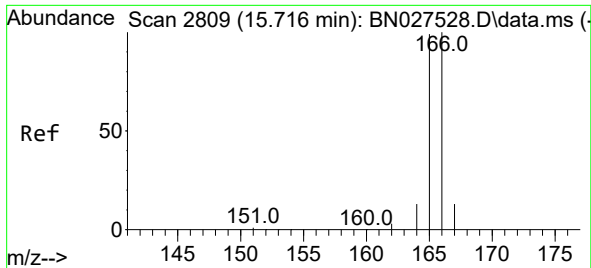

#12
Fluorene
Concen: 0.050 ng/ul
RT: 15.660 min Scan# 21
Delta R.T. -0.065 min
Lab File: BN027546.D
Acq: 10 Sep 2023 18:29




Instrument :
BNA_N
ClientSampleId :
SBLK348


Tgt Ion:166 Resp: 3095
Ion Ratio Lower Upper
166 100
165 8.6 79.6 119.4#
167 35.6 11.4 17.0#

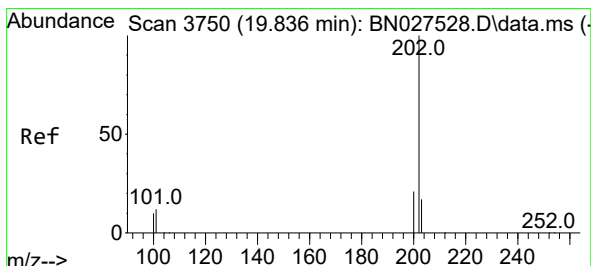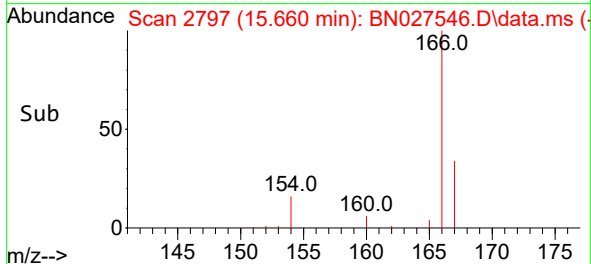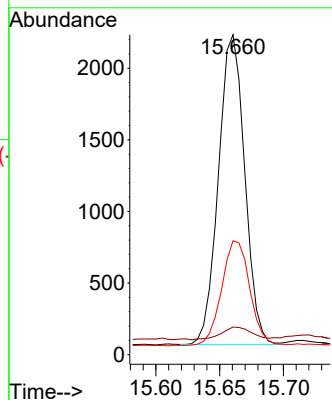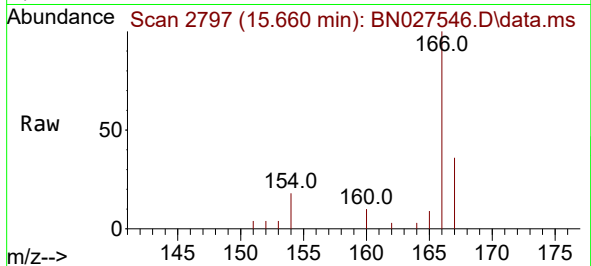

#20
Pyrene
Concen: 0.030 ng/ul
RT: 19.808 min Scan# 3744
Delta R.T. -0.033 min
Lab File: BN027546.D
Acq: 10 Sep 2023 18:29


Tgt Ion:202 Resp: 2664
Ion Ratio Lower Upper
202 100
101 152.4 11.4 17.2#
100 1070.5 9.4 14.2#

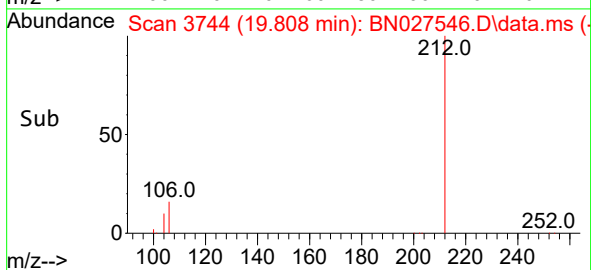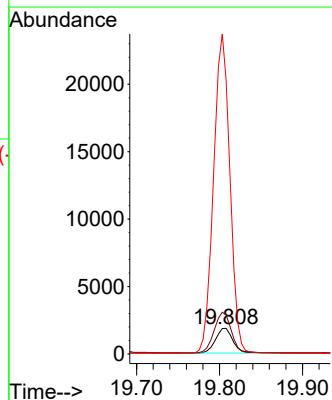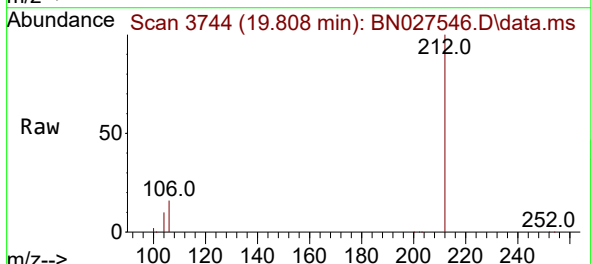

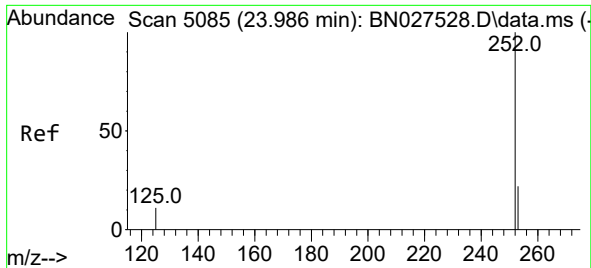

#26
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.933 min Scan# 50
Delta R.T. -0.062 min
Lab File: BN027546.D
Acq: 10 Sep 2023 18:29

Instrument :
BNA_N
ClientSampleId :
SBLK348

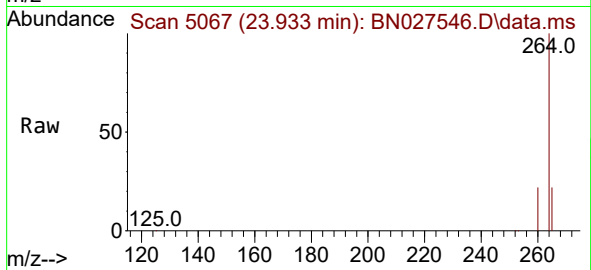

Tgt Ion:252 Resp: 4284
Ion Ratio Lower Upper
252 100
253 52.6 22.4 33.6#
125 47.2 17.4 26.2#

