

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027549.D
 Acq On : 10 Sep 2023 20:20
 Operator : MA/JU
 Sample : 04262-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJD4

Quant Time: Sep 11 01:20:47 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	5829	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136	20122	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	12145	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.418	188	26970	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	19861	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	18393	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	39195	5.055	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	9775	0.320	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	26055	0.383	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	195	0.025	ng/ul#	48
20) Pyrene	19.804	202	3700	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.936	252	6382	0.094	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027549.D
Acq On : 10 Sep 2023 20:20
Operator : MA/JU
Sample : 04262-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJD4

Quant Time: Sep 11 01:20:47 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




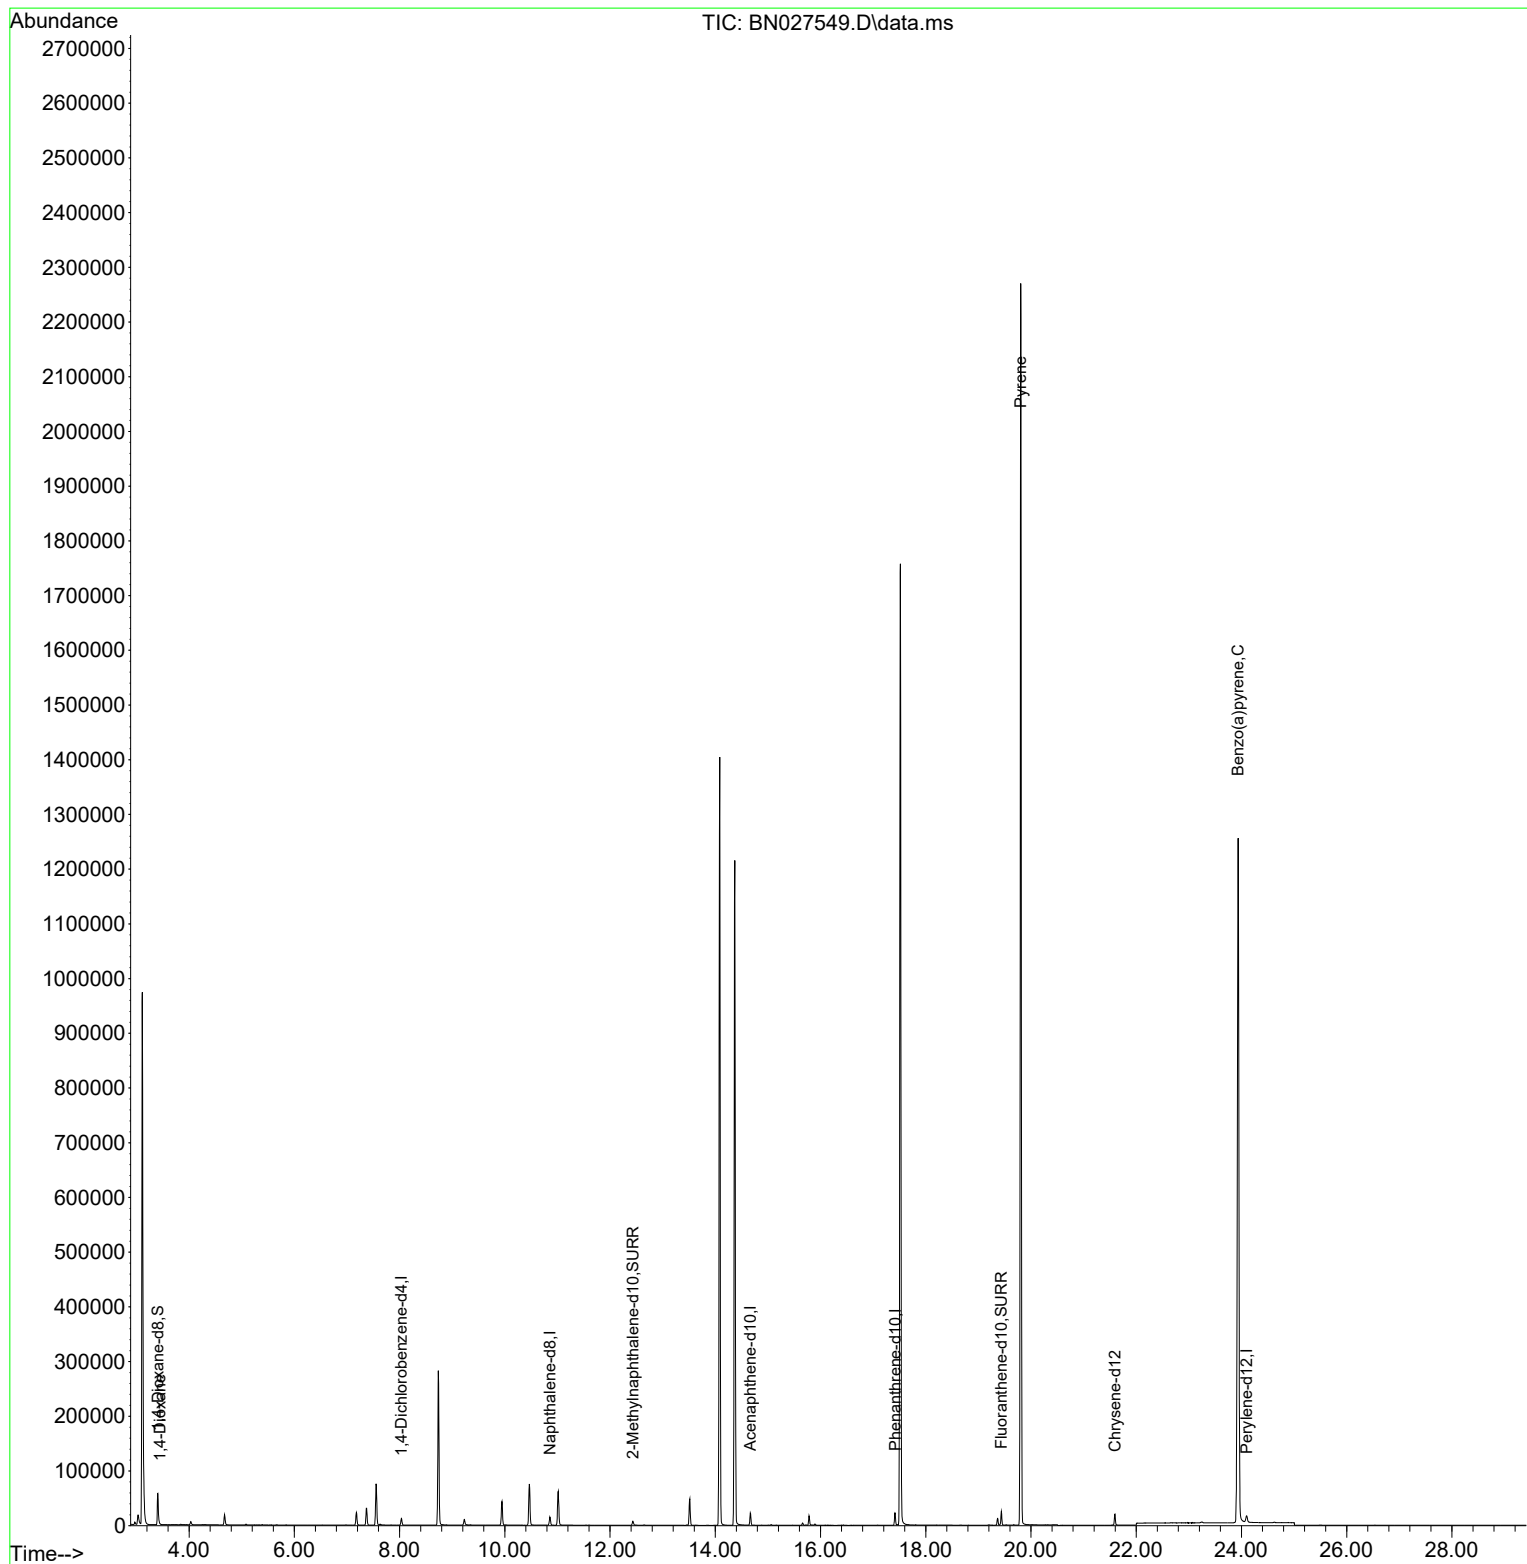


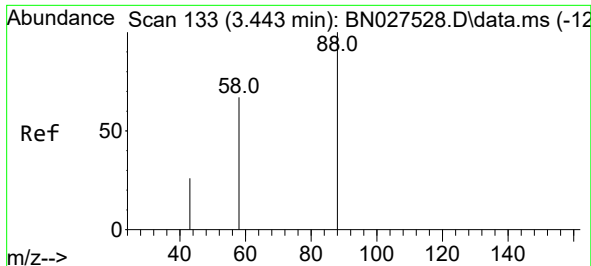

#2
1,4-Dioxane
Concen: 0.025 ng/ul
RT: 3.444 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027549.D
Acq: 10 Sep 2023 20:20




Instrument :
BNA_N
ClientSampleId :
BBJD4


Tgt Ion: 88 Resp: 195
Ion Ratio Lower Upper
88 100
43 91.6 26.8 40.2#
58 36.7 39.9 59.9#

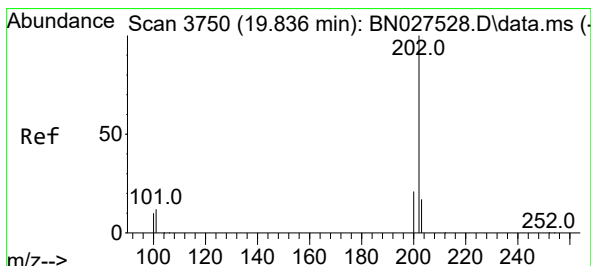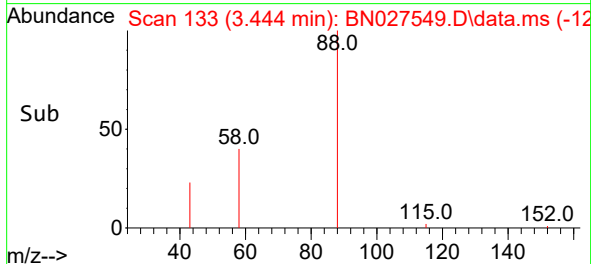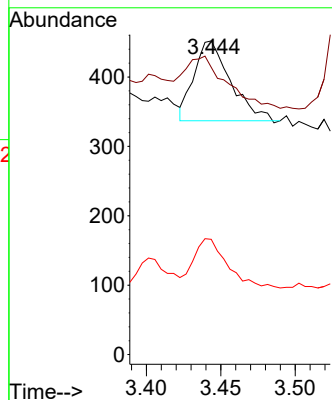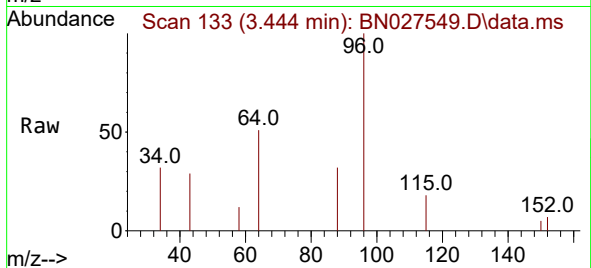

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.804 min Scan# 3743
Delta R.T. -0.037 min
Lab File: BN027549.D
Acq: 10 Sep 2023 20:20


Tgt Ion: 202 Resp: 3700
Ion Ratio Lower Upper
202 100
101 156.8 11.4 17.2#
100 1183.6 9.4 14.2#

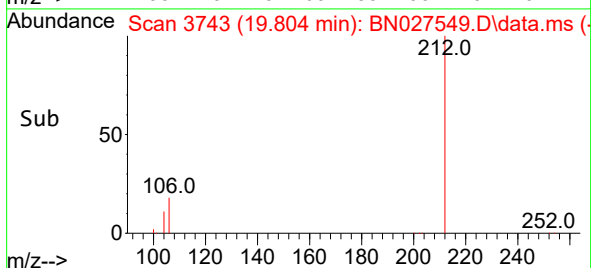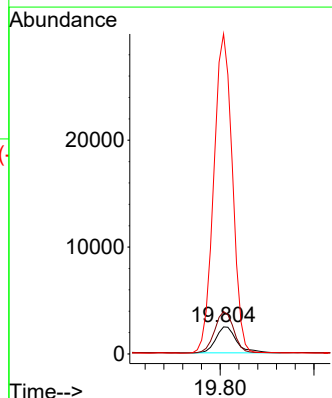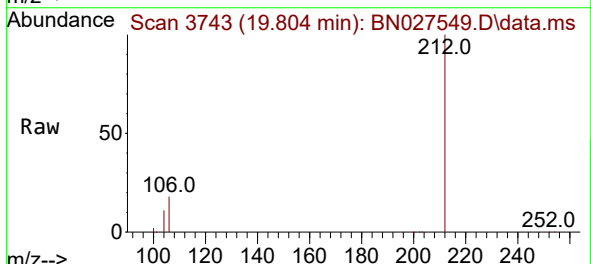

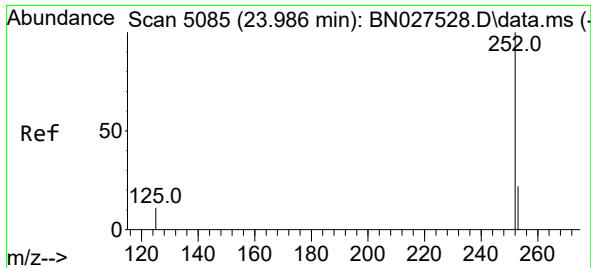

#26
Benzo(a)pyrene
Concen: 0.094 ng/ul
RT: 23.936 min Scan# 50
Delta R.T. -0.058 min
Lab File: BN027549.D
Acq: 10 Sep 2023 20:20

Instrument :
BNA_N
ClientSampleId :
BBJD4

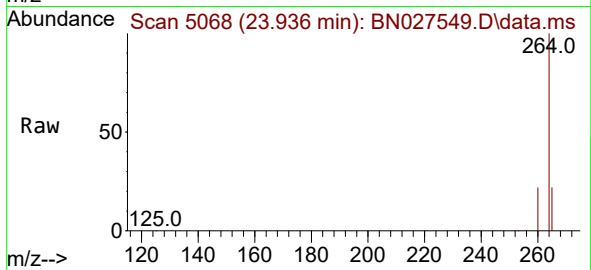

Tgt Ion:252 Resp: 6382
Ion Ratio Lower Upper
252 100
253 46.1 22.4 33.6#
125 39.3 17.4 26.2#

