

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027552.D
 Acq On : 10 Sep 2023 22:11
 Operator : MA/JU
 Sample : 04262-06
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBHM8

Quant Time: Sep 11 01:21:05 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	7446	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136	25744	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	15361	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.413	188	33396	0.400	ng/ul	-0.01
17) Chrysene-d12	21.589	240	23812	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	20896	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	41013	4.141	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	11011	0.282	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	29903	0.367	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.443	88	363	0.036	ng/ul#	55
20) Pyrene	19.803	202	5194	0.047	ng/ul#	1
26) Benzo(a)pyrene	23.933	252	6950	0.090	ng/ul#	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027552.D
Acq On : 10 Sep 2023 22:11
Operator : MA/JU
Sample : 04262-06
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBHM8

Quant Time: Sep 11 01:21:05 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




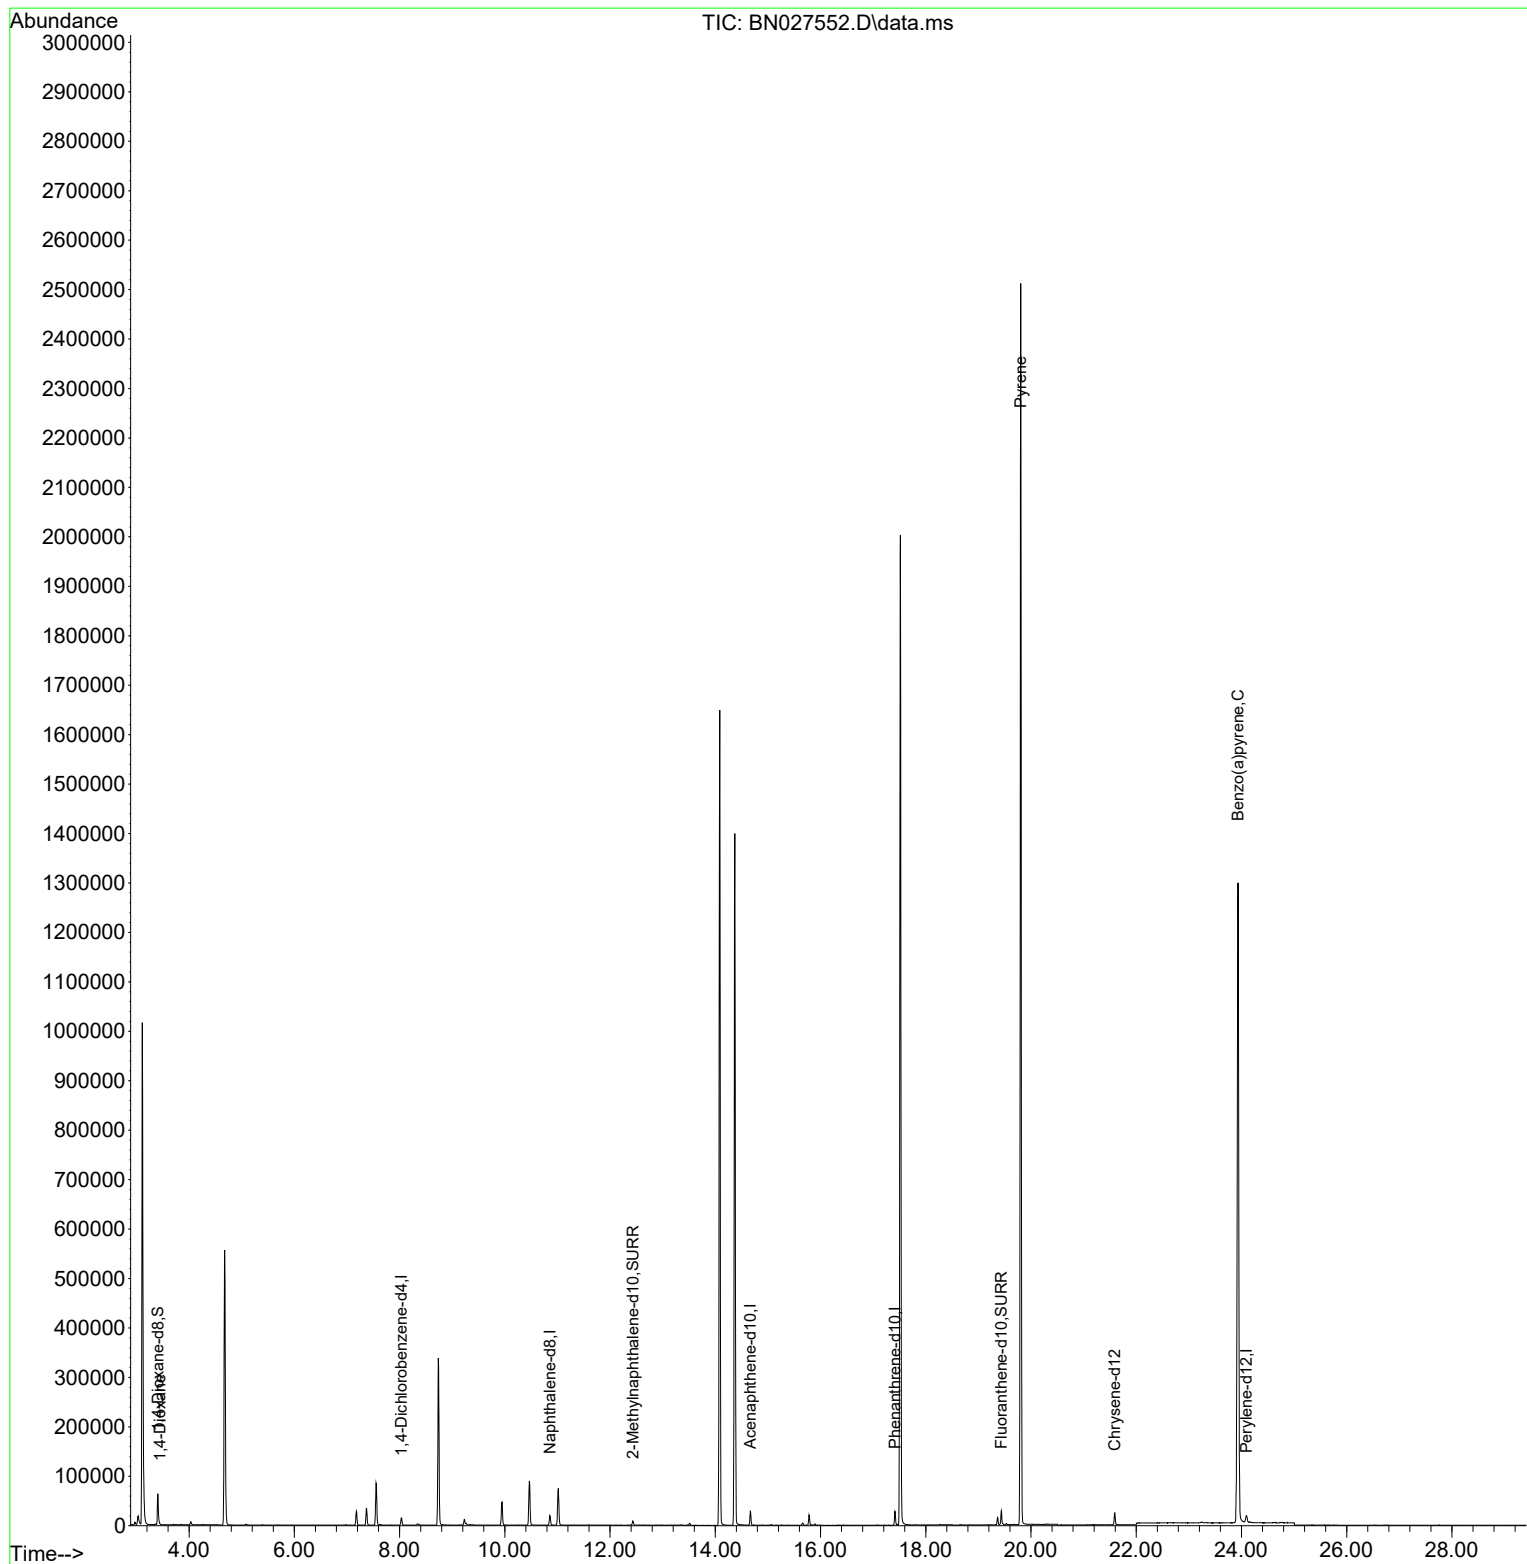


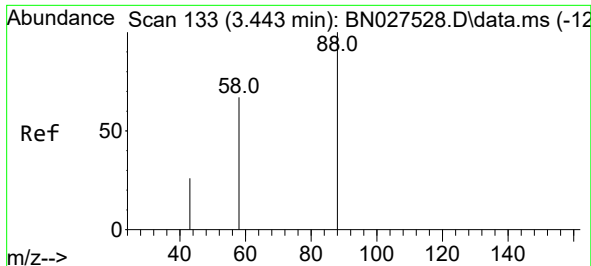

#2
1,4-Dioxane
Concen: 0.036 ng/ul
RT: 3.443 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027552.D
Acq: 10 Sep 2023 22:11




Instrument :
BNA_N
ClientSampleId :
BBHM8


Tgt Ion: 88 Resp: 363
Ion Ratio Lower Upper
88 100
43 85.3 26.8 40.2#
58 40.5 39.9 59.9

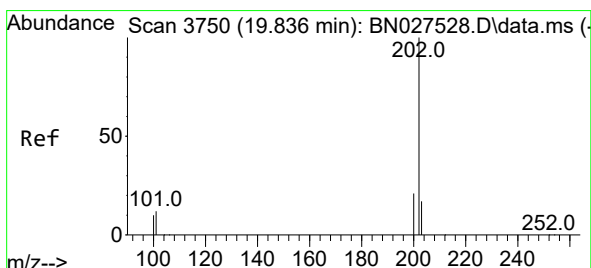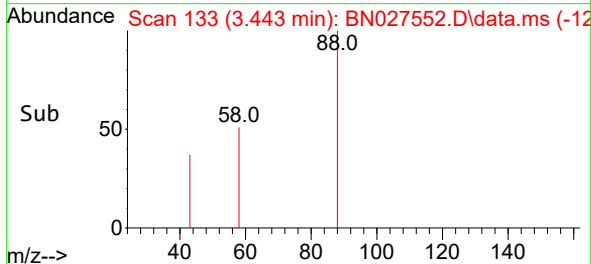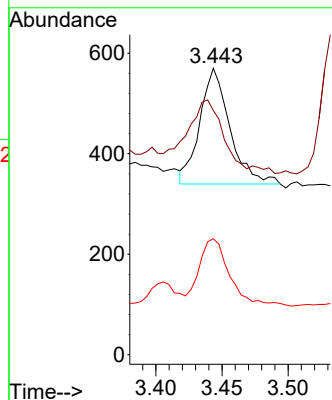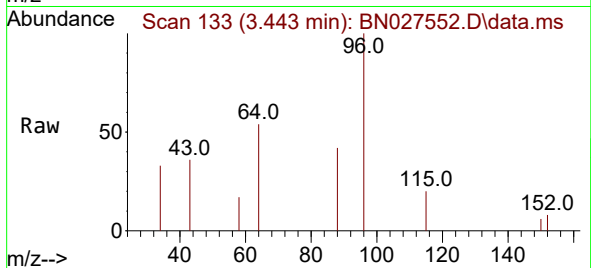

#20
Pyrene
Concen: 0.047 ng/ul
RT: 19.803 min Scan# 3743
Delta R.T. -0.037 min
Lab File: BN027552.D
Acq: 10 Sep 2023 22:11

Tgt Ion: 202 Resp: 5194
Ion Ratio Lower Upper
202 100
101 151.3 11.4 17.2#
100 1120.1 9.4 14.2#

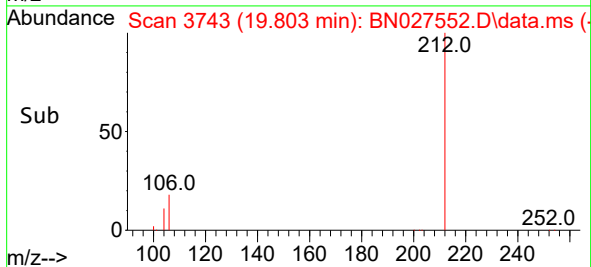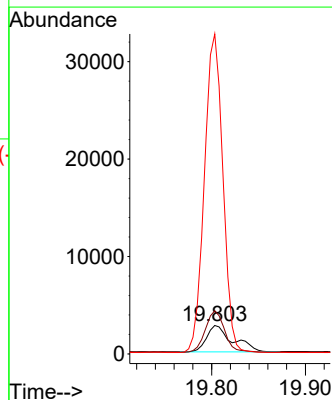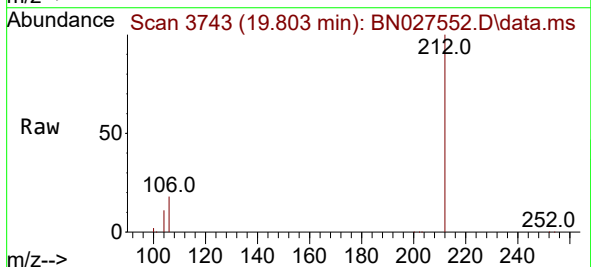

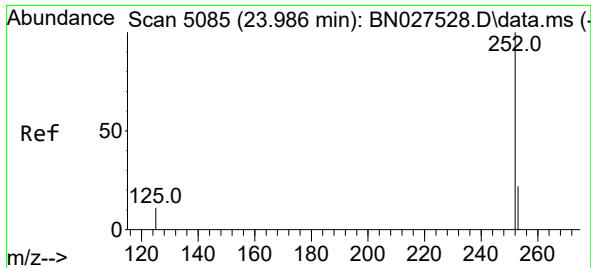

#26

Benzo(a)pyrene

Concen: 0.090 ng/ul

RT: 23.933 min Scan# 50

Delta R.T. -0.062 min

Lab File: BN027552.D


Acq: 10 Sep 2023 22:11

Instrument :

BNA_N

ClientSampleId :

BBHM8

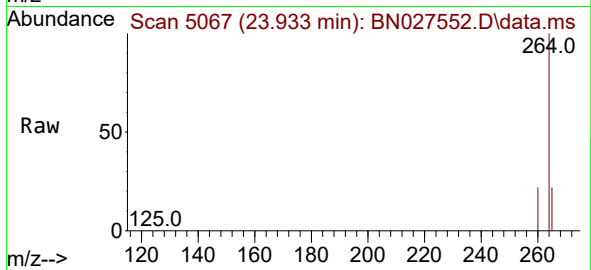

Tgt Ion:252 Resp: 6950

Ion Ratio Lower Upper

252 100

253 48.6 22.4 33.6#

125 42.7 17.4 26.2#

