

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027554.D
 Acq On : 10 Sep 2023 23:24
 Operator : MA/JU
 Sample : 04268-01
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0GH1

Quant Time: Sep 11 01:21:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	6416	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136	22225	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	13290	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.418	188	28496	0.400	ng/ul	0.00
17) Chrysene-d12	21.589	240	19700	0.400	ng/ul	0.00
23) Perylene-d12	24.091	264	17648	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	30933	3.624	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	9226	0.274	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	26541	0.393	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	3824	0.041	ng/ul#	1
26) Benzo(a)pyrene	23.930	252	6292	0.097	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027554.D
Acq On : 10 Sep 2023 23:24
Operator : MA/JU
Sample : 04268-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0GH1

Quant Time: Sep 11 01:21:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

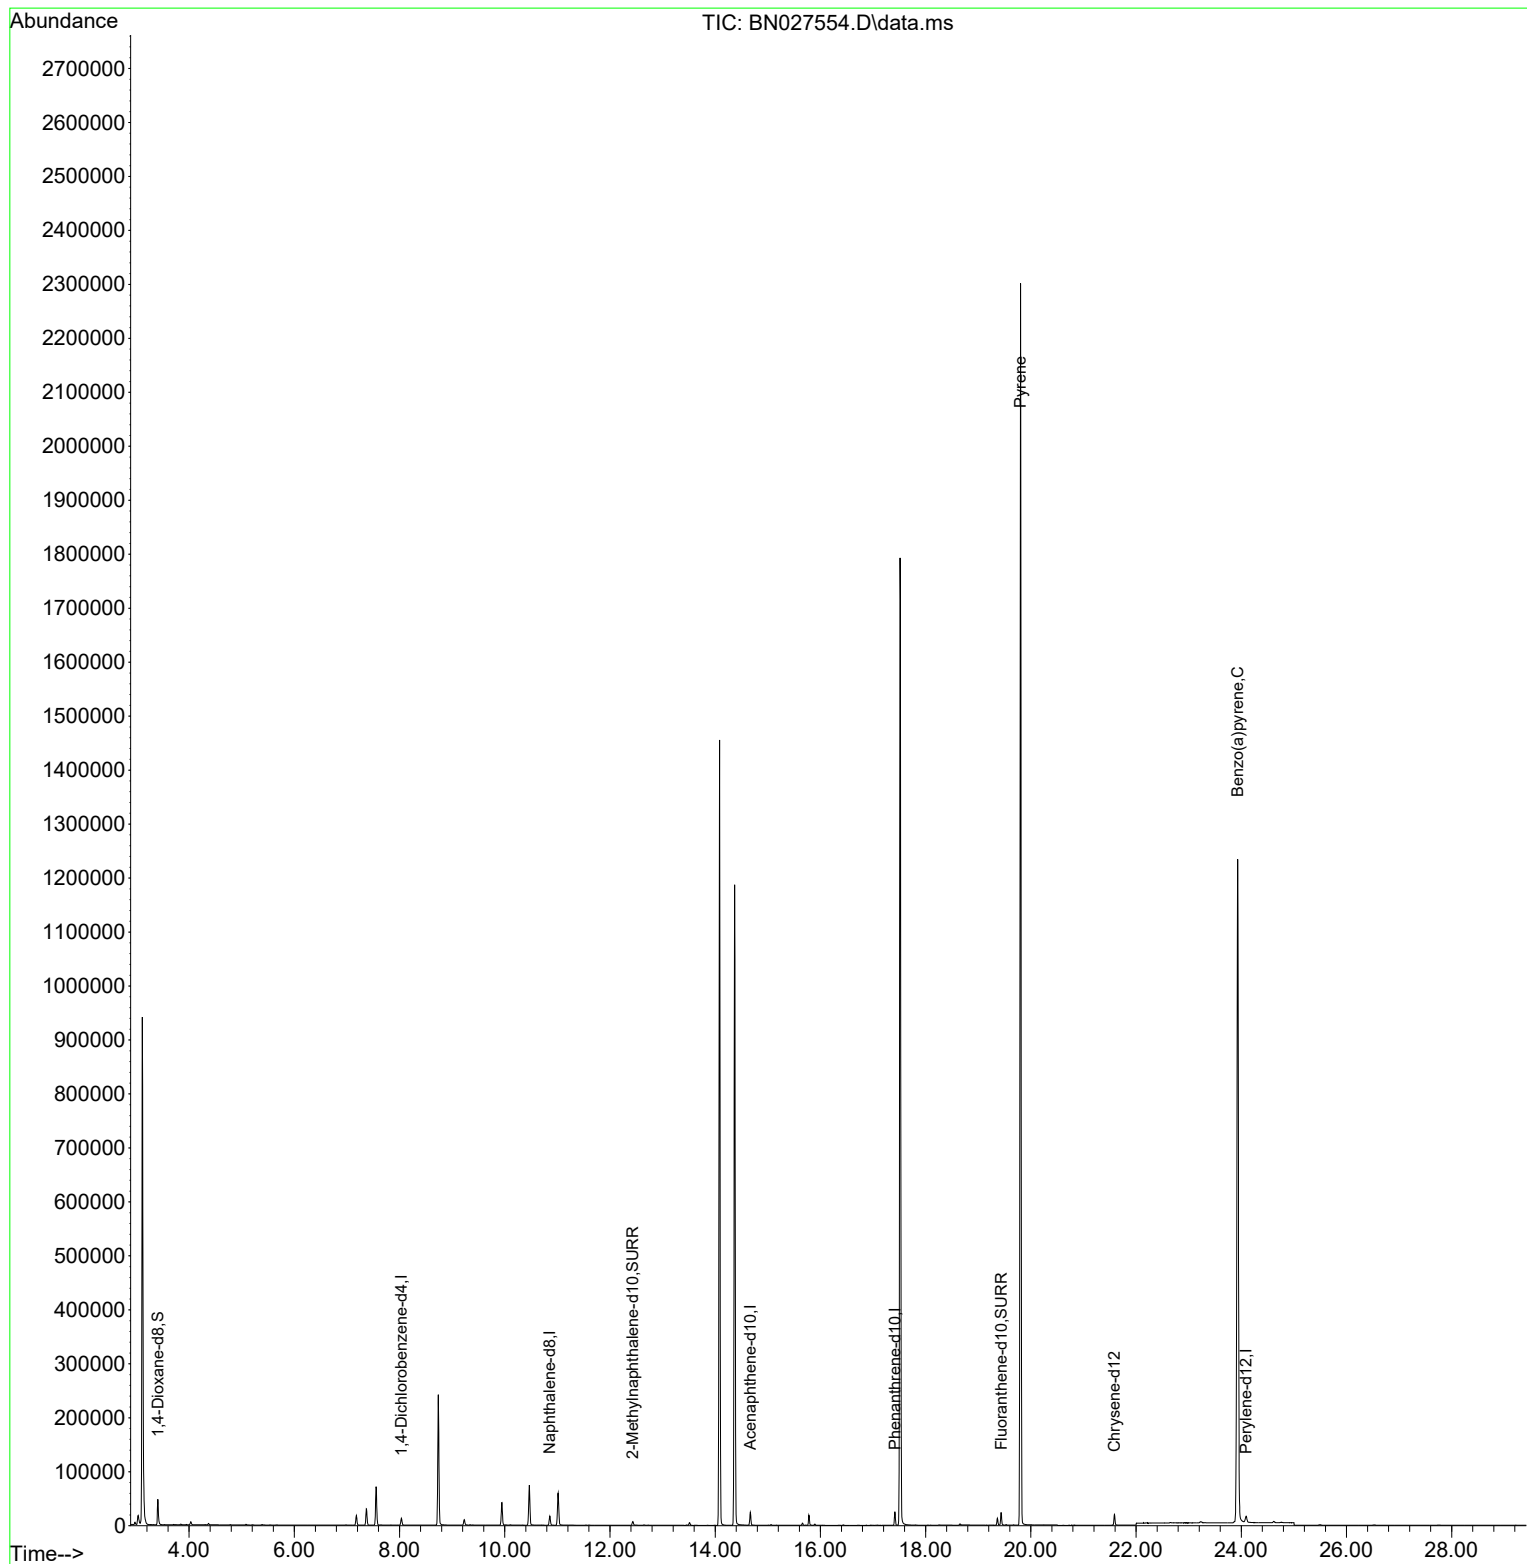

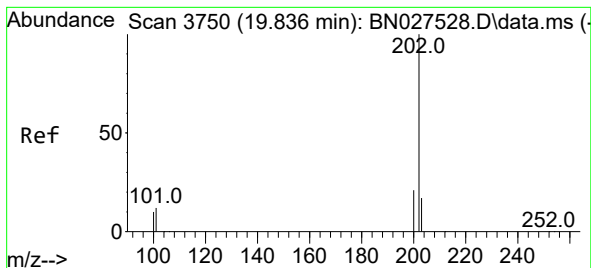

#20

Pyrene

Concen: 0.041 ng/ul

RT: 19.803 min Scan# 31

Delta R.T. -0.037 min

Lab File: BN027554.D

Acq: 10 Sep 2023 23:24

Instrument :

BNA_N

ClientSampleId :

H0GH1





Tgt Ion:202 Resp: 3824

Ion Ratio Lower Upper

202 100

101 158.5 11.4 17.2#

100 1190.8 9.4 14.2#

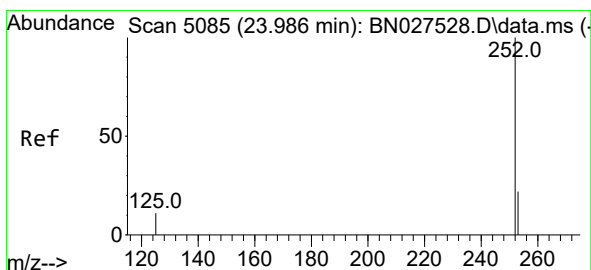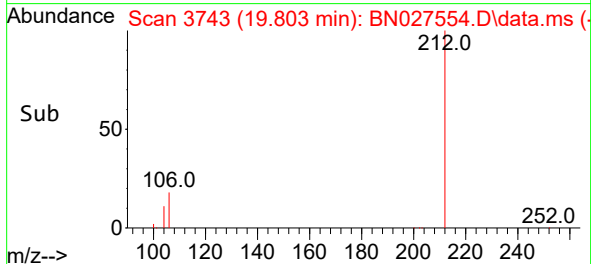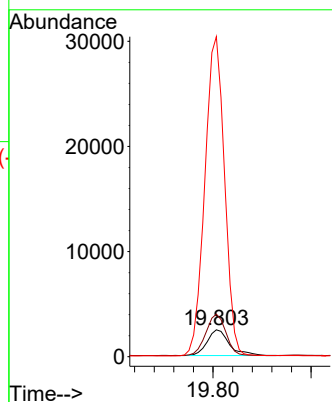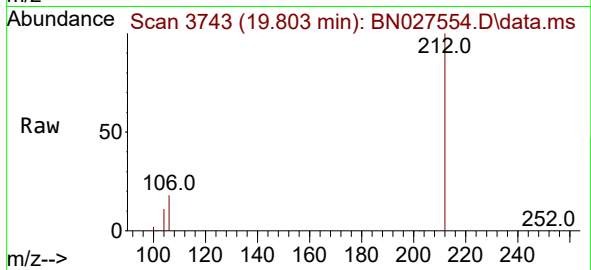

#26

Benzo(a)pyrene

Concen: 0.097 ng/ul

RT: 23.930 min Scan# 5066

Delta R.T. -0.064 min

Lab File: BN027554.D

Acq: 10 Sep 2023 23:24

Tgt Ion:252 Resp: 6292

Ion Ratio Lower Upper

252 100

253 46.8 22.4 33.6#

125 41.2 17.4 26.2#

