

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027556.D
 Acq On : 11 Sep 2023 00:38
 Operator : MA/JU
 Sample : 04268-06
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 H0GH4

Quant Time: Sep 11 01:21:30 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	6570	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136	22532	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	13362	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.417	188	28680	0.400	ng/ul	0.00
17) Chrysene-d12	21.591	240	19598	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	17330	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	30827	3.527	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	9809	0.287	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	25783	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.803	202	3573	0.039	ng/ul#	1
26) Benzo(a)pyrene	23.930	252	5709	0.089	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027556.D
Acq On : 11 Sep 2023 00:38
Operator : MA/JU
Sample : 04268-06
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
H0GH4

Quant Time: Sep 11 01:21:30 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

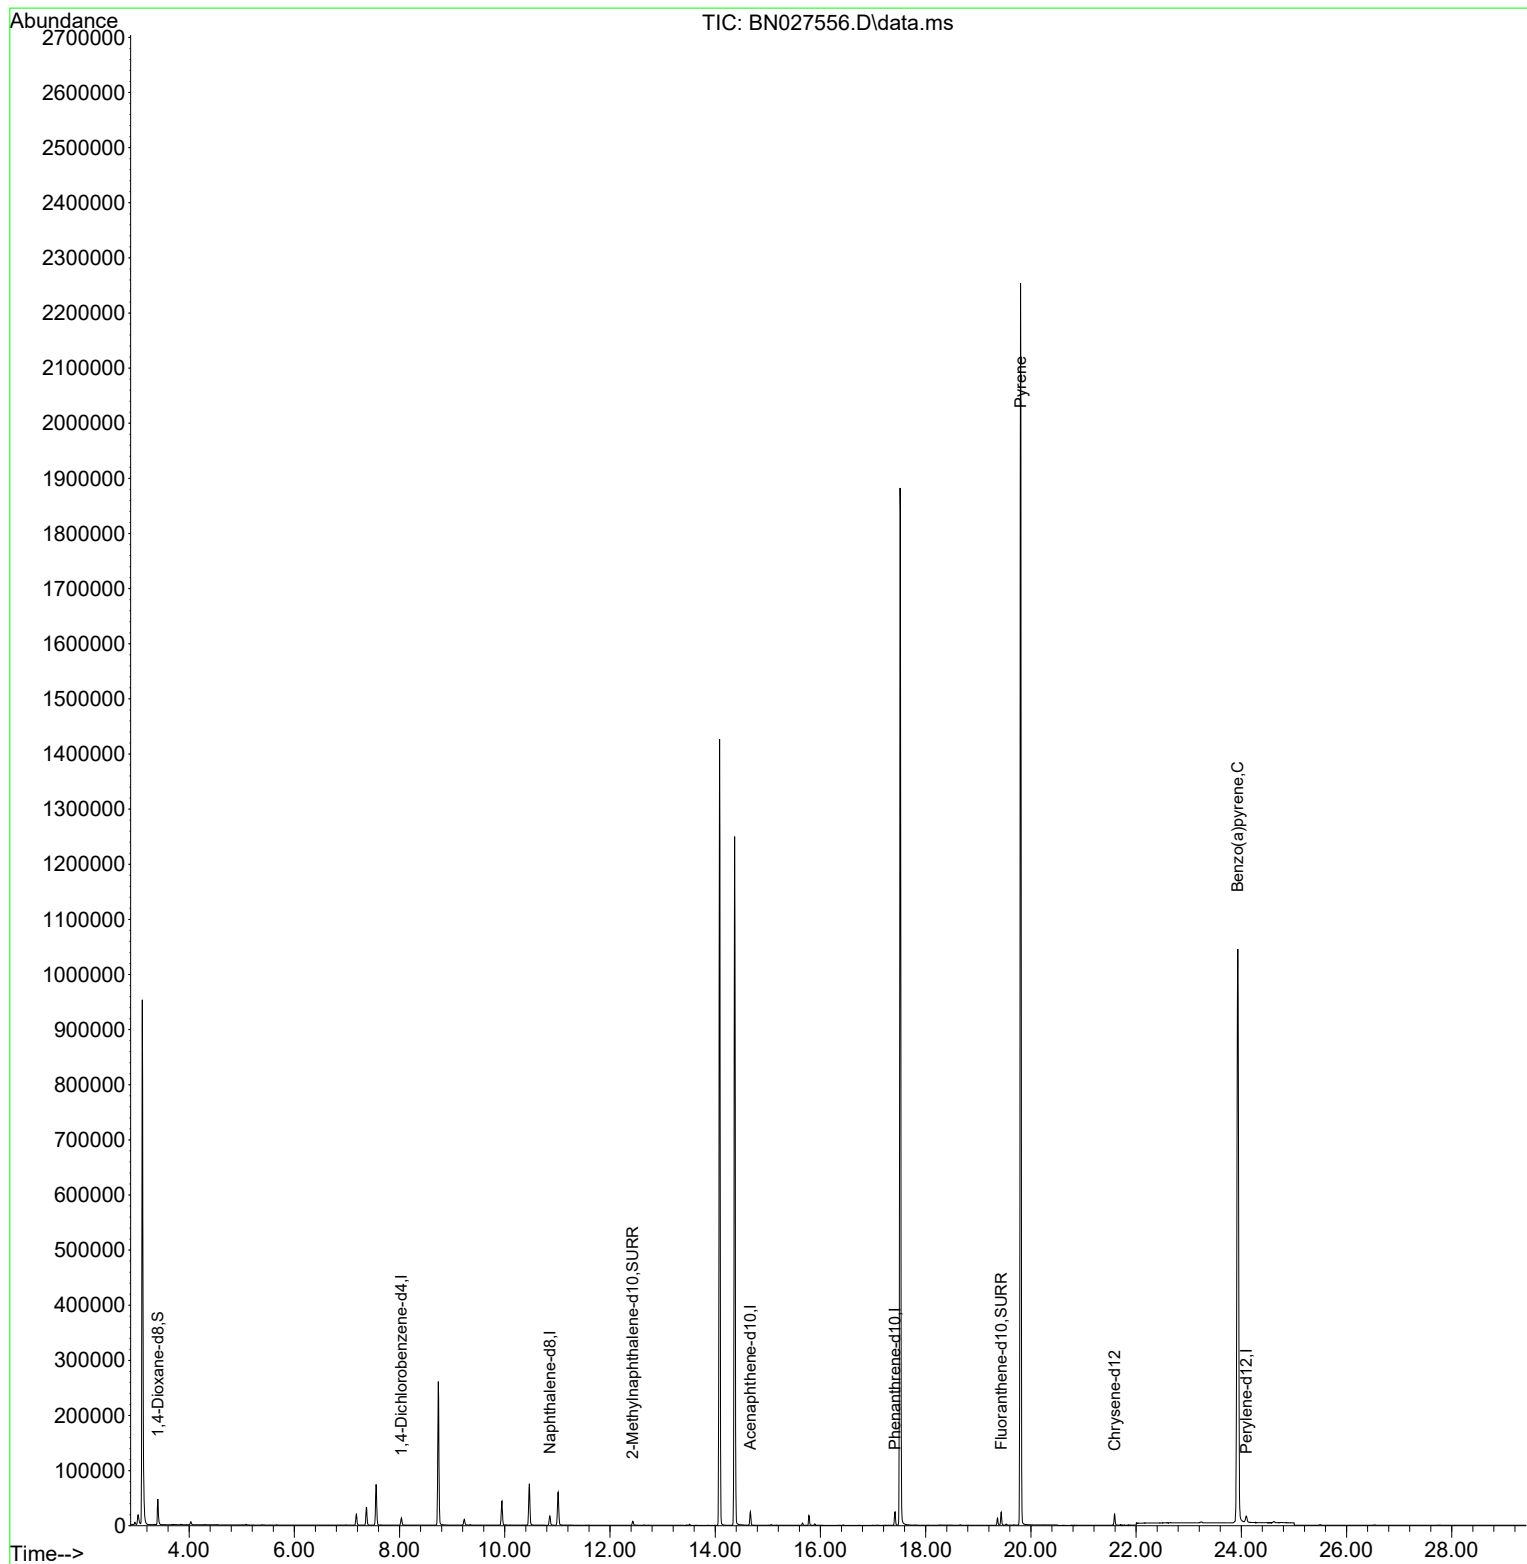

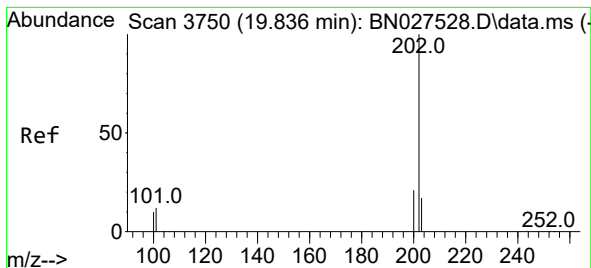

#20

Pyrene

Concen: 0.039 ng/ul

RT: 19.803 min Scan# 31

Delta R.T. -0.038 min

Lab File: BN027556.D

Acq: 11 Sep 2023 00:38

Instrument :

BNA_N

ClientSampleId :

H0GH4





Tgt Ion:202 Resp: 3573

Ion Ratio Lower Upper

202 100

101 156.8 11.4 17.2#

100 1171.7 9.4 14.2#

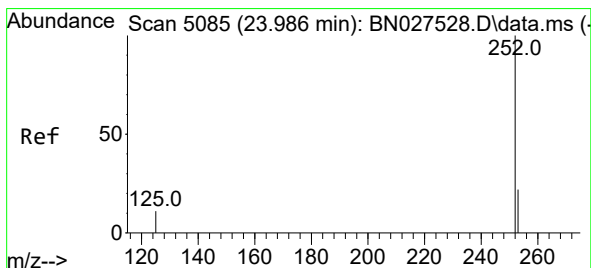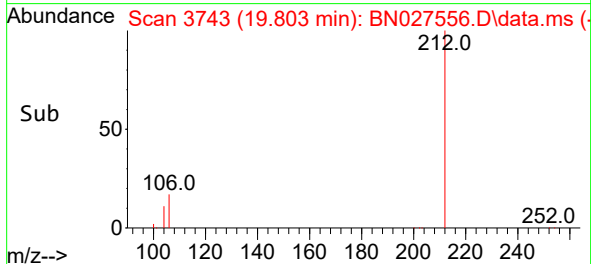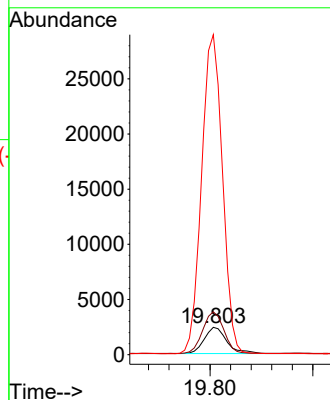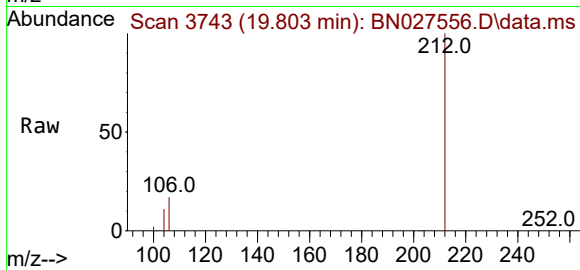

#26

Benzo(a)pyrene

Concen: 0.089 ng/ul

RT: 23.930 min Scan# 5066

Delta R.T. -0.065 min

Lab File: BN027556.D

Acq: 11 Sep 2023 00:38

Tgt Ion:252 Resp: 5709

Ion Ratio Lower Upper

252 100

253 49.4 22.4 33.6#

125 44.3 17.4 26.2#

