




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027534.D
Acq On : 10 Sep 2023 11:08
Operator : MA/JU
Sample : 04250-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH4A3

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:18:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

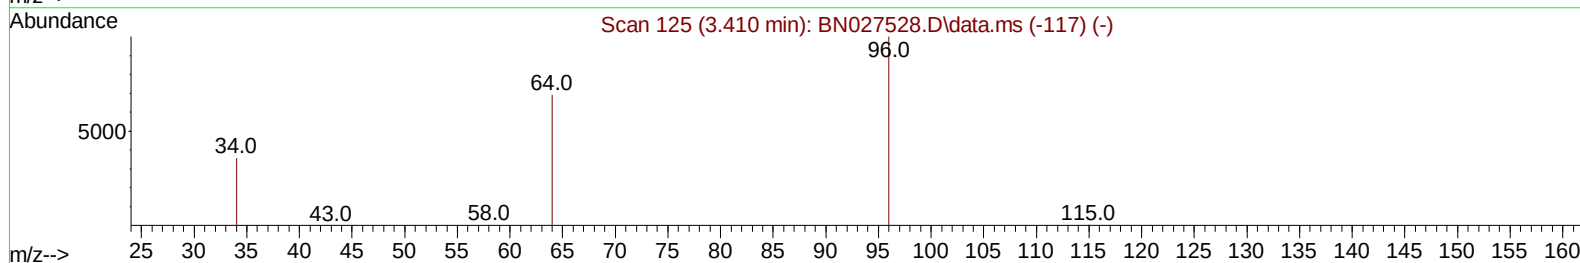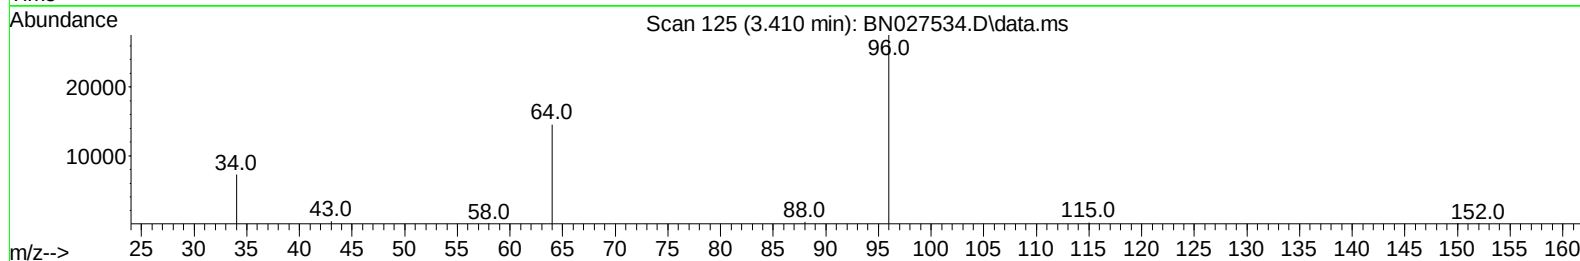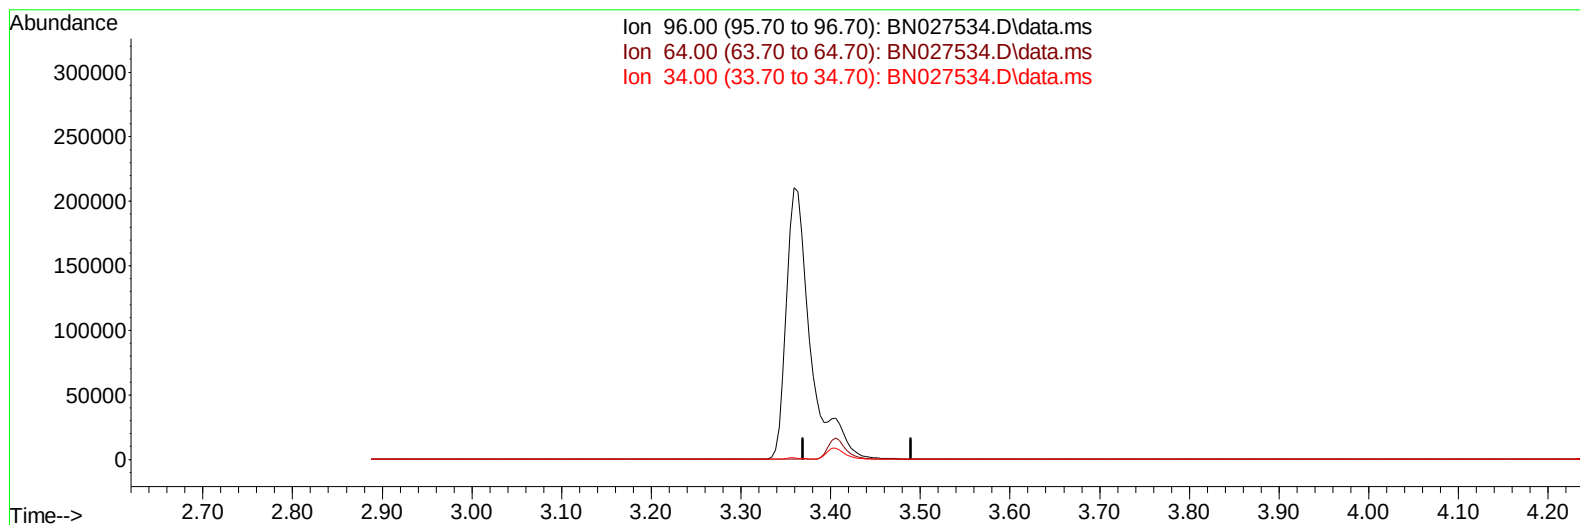

TIC: BN027534.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.410min (-3.410) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	53.80	0.00#
34.00	36.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027534.D
 Acq On : 10 Sep 2023 11:08
 Operator : MA/JU
 Sample : 04250-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4A3

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:18:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

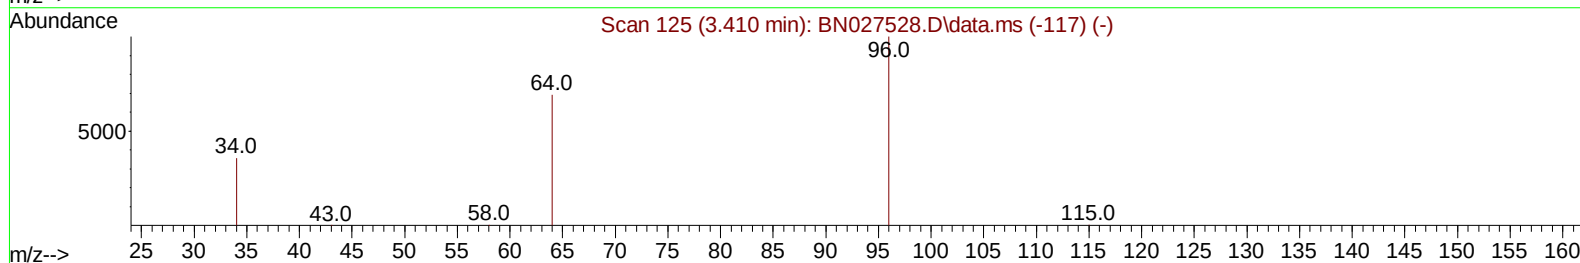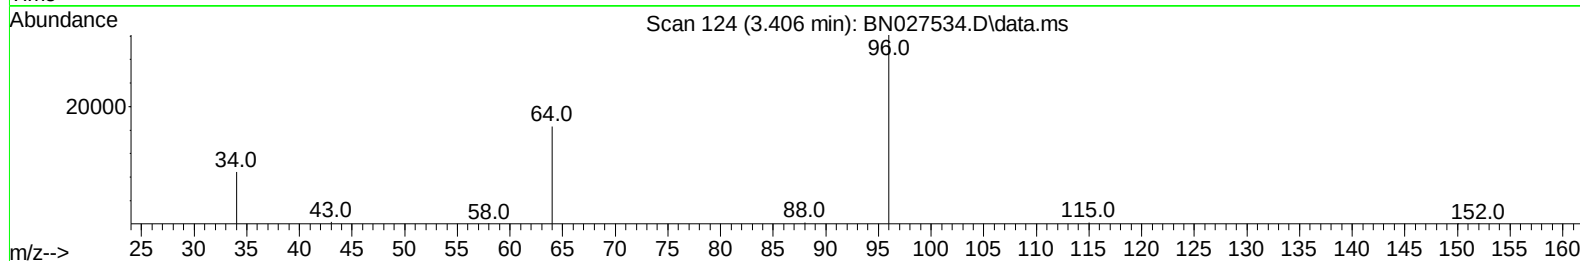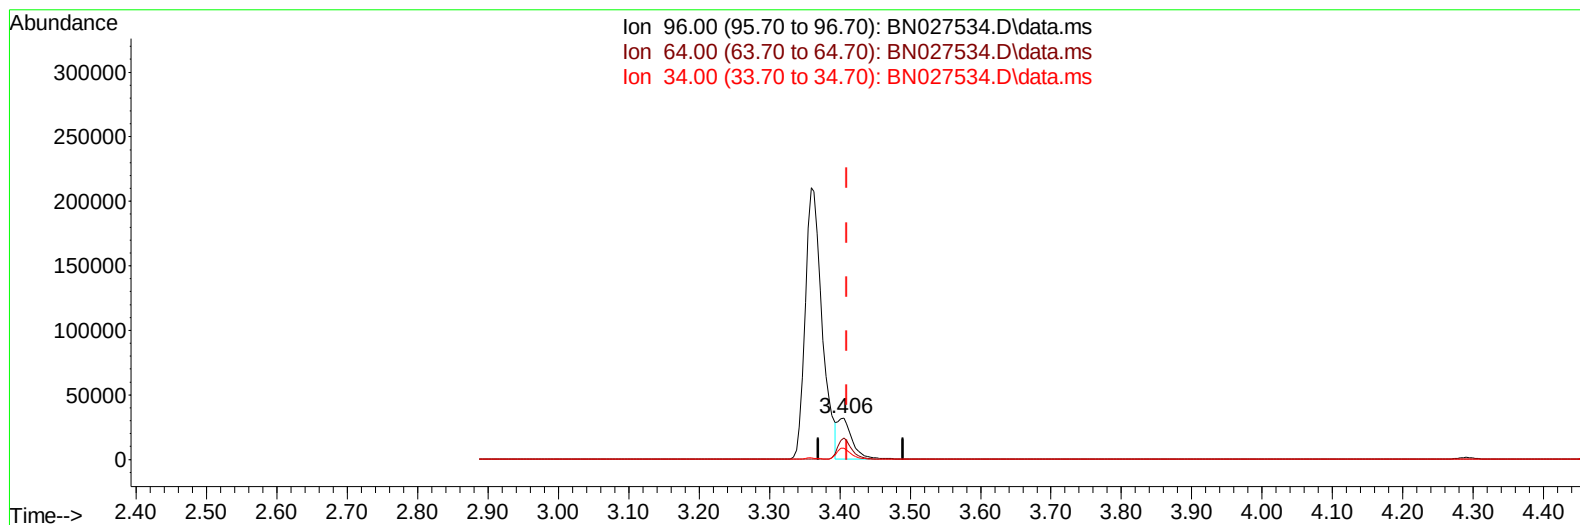

TIC: BN027534.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.406min (-0.004) 5.33 ng/ul m

response 46168

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	53.80	51.68
34.00	36.40	27.50#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027534.D
 Acq On : 10 Sep 2023 11:08
 Operator : MA/JU
 Sample : 04250-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4A3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 11 01:18:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.038	152		6508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136		22539	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164		14158	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.418	188		31274	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240		21467	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264		20130	0.400	ng/ul	#-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.406	96		46168m	5.333	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152		12488	0.365	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212		30488	0.415	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.444	88		1376	0.157	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027534.D
Acq On : 10 Sep 2023 11:08
Operator : MA/JU
Sample : 04250-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH4A3

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:18:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

