




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027536.D
 Acq On : 10 Sep 2023 12:21
 Operator : MA/JU
 Sample : 04250-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4E8

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:18:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

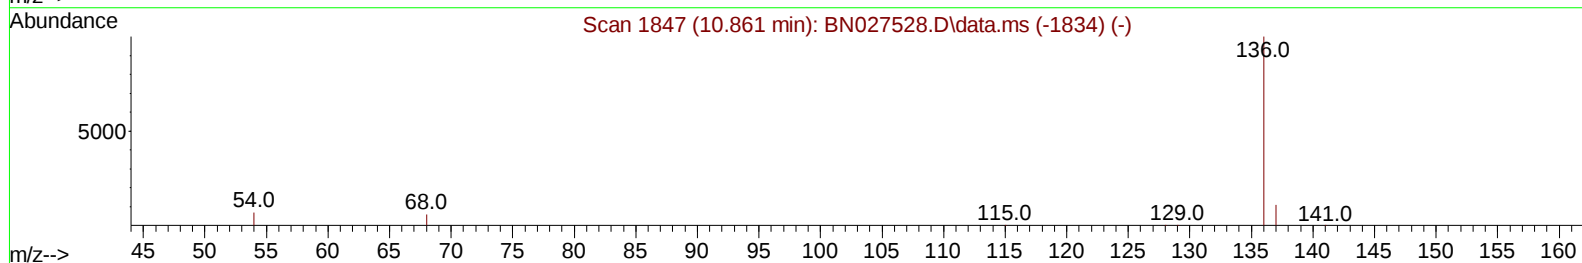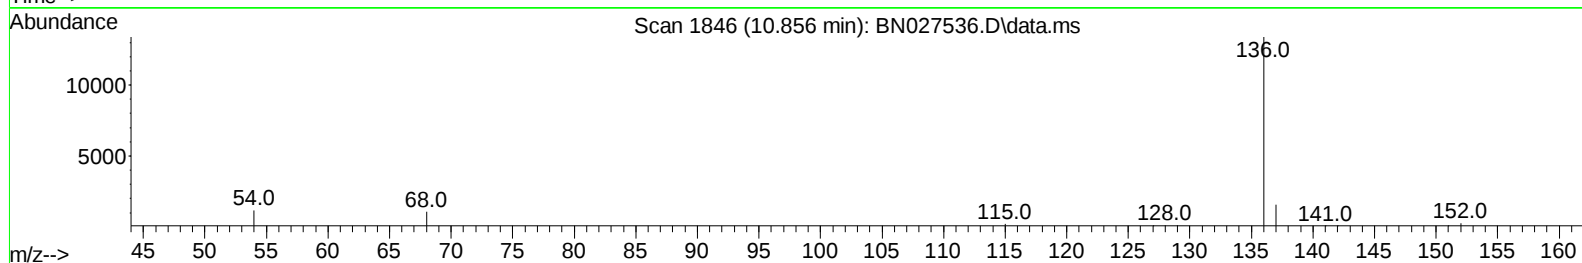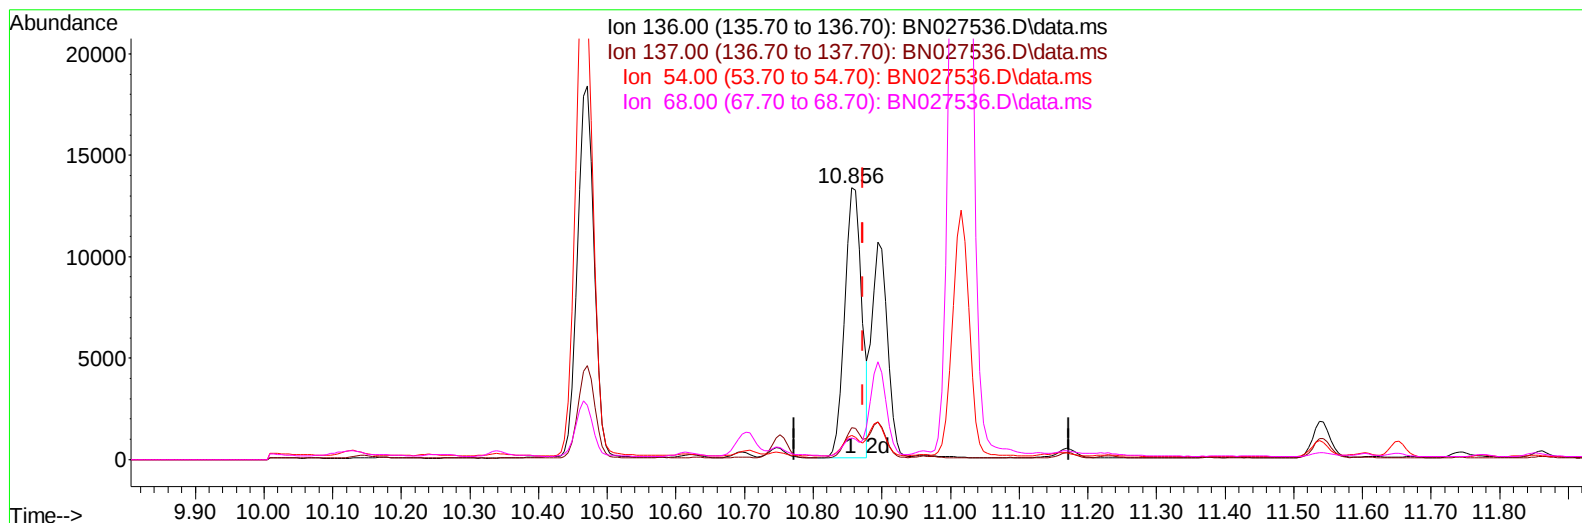

TIC: BN027536.D\data.ms

(4) Naphthalene-d8 (I)

10.856min (-0.017) 0.40 ng/u1

response 23143

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.80	11.60
54.00	8.50	8.83
68.00	7.20	7.94




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027536.D
 Acq On : 10 Sep 2023 12:21
 Operator : MA/JU
 Sample : 04250-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4E8

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:18:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

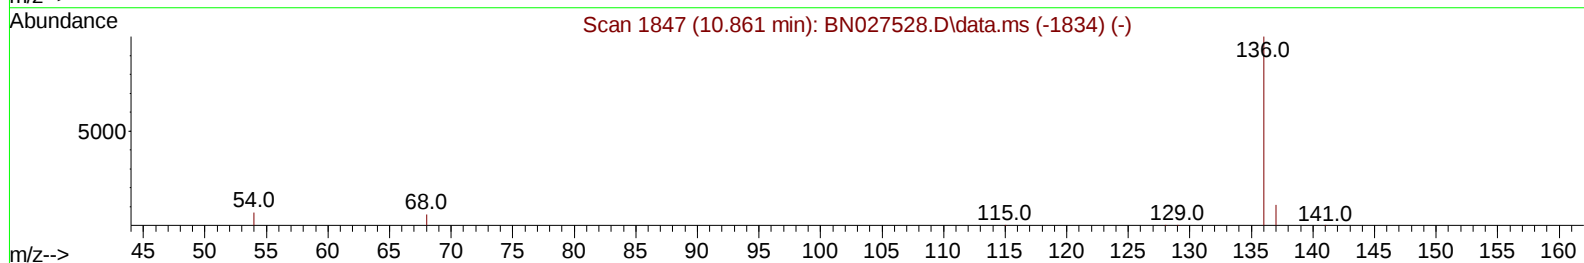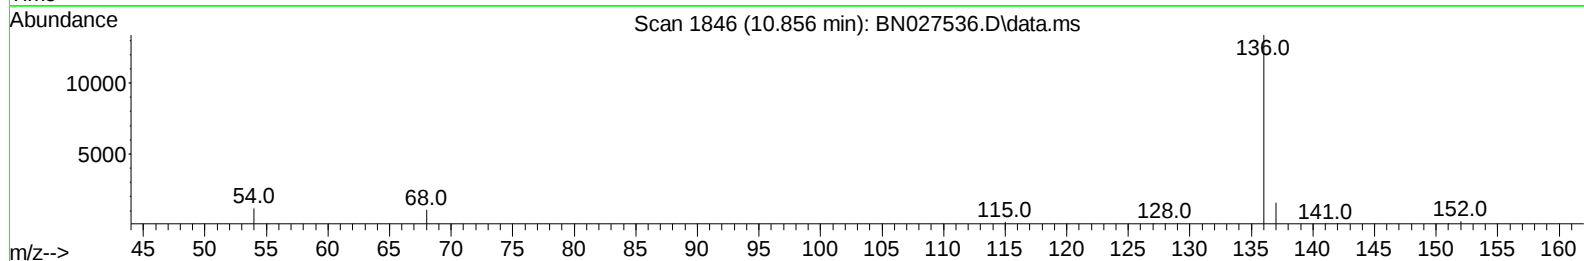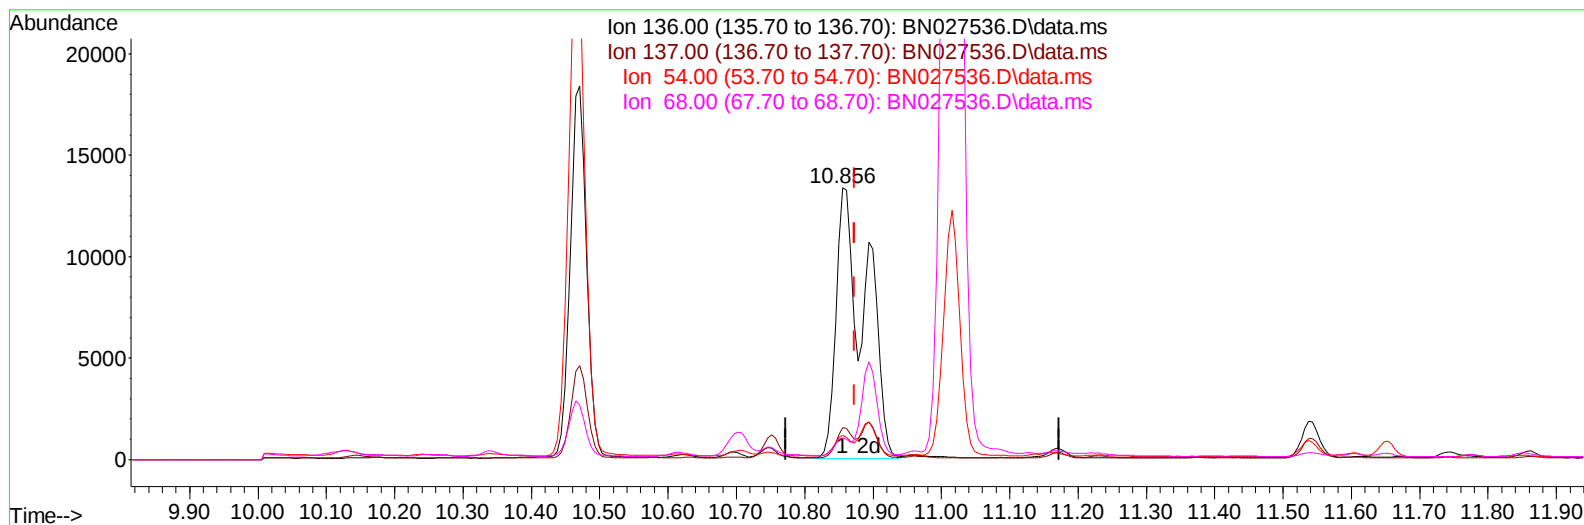

TIC: BN027536.D\data.ms

(4) Naphthalene-d8 (I)

10.856min (-0.017) 0.40 ng/ul m

response 39947

Ion	Exp%	Act%
136.00	100.00	100.00
137.00	11.80	11.60
54.00	8.50	8.83
68.00	7.20	7.94

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027536.D
 Acq On : 10 Sep 2023 12:21
 Operator : MA/JU
 Sample : 04250-11
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4E8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 11 01:18:52 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.034	152		6587	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136		39947m	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.670	164		14675	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.417	188		30740	0.400	ng/ul	0.00
17) Chrysene-d12	21.597	240		21078	0.400	ng/ul	0.00
23) Perylene-d12	24.103	264		19552	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.405	96		46235	5.277	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152		13752	0.227	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212		31646	0.438	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027536.D
Acq On : 10 Sep 2023 12:21
Operator : MA/JU
Sample : 04250-11
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH4E8

Manual IntegrationsAPPROVED

Quant Time: Sep 11 01:18:52 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

