

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027508.D
 Acq On : 09 Sep 2023 19:04
 Operator : MA/JU
 Sample : 04227-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJW6

Quant Time: Sep 10 00:12:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	10682	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	36997	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.675	164	24421	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	51420	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.594	240	37031	0.400	ng/ul	0.00
23) Perylene-d12	24.103	264	34371	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	51155	3.600	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	24603	0.438	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	57864	0.456	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.448	88	7056	0.491	ng/ul#	88
14) Pentachlorophenol	17.054	266	12410	1.238	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027508.D
Acq On : 09 Sep 2023 19:04
Operator : MA/JU
Sample : 04227-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJW6

Quant Time: Sep 10 00:12:40 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




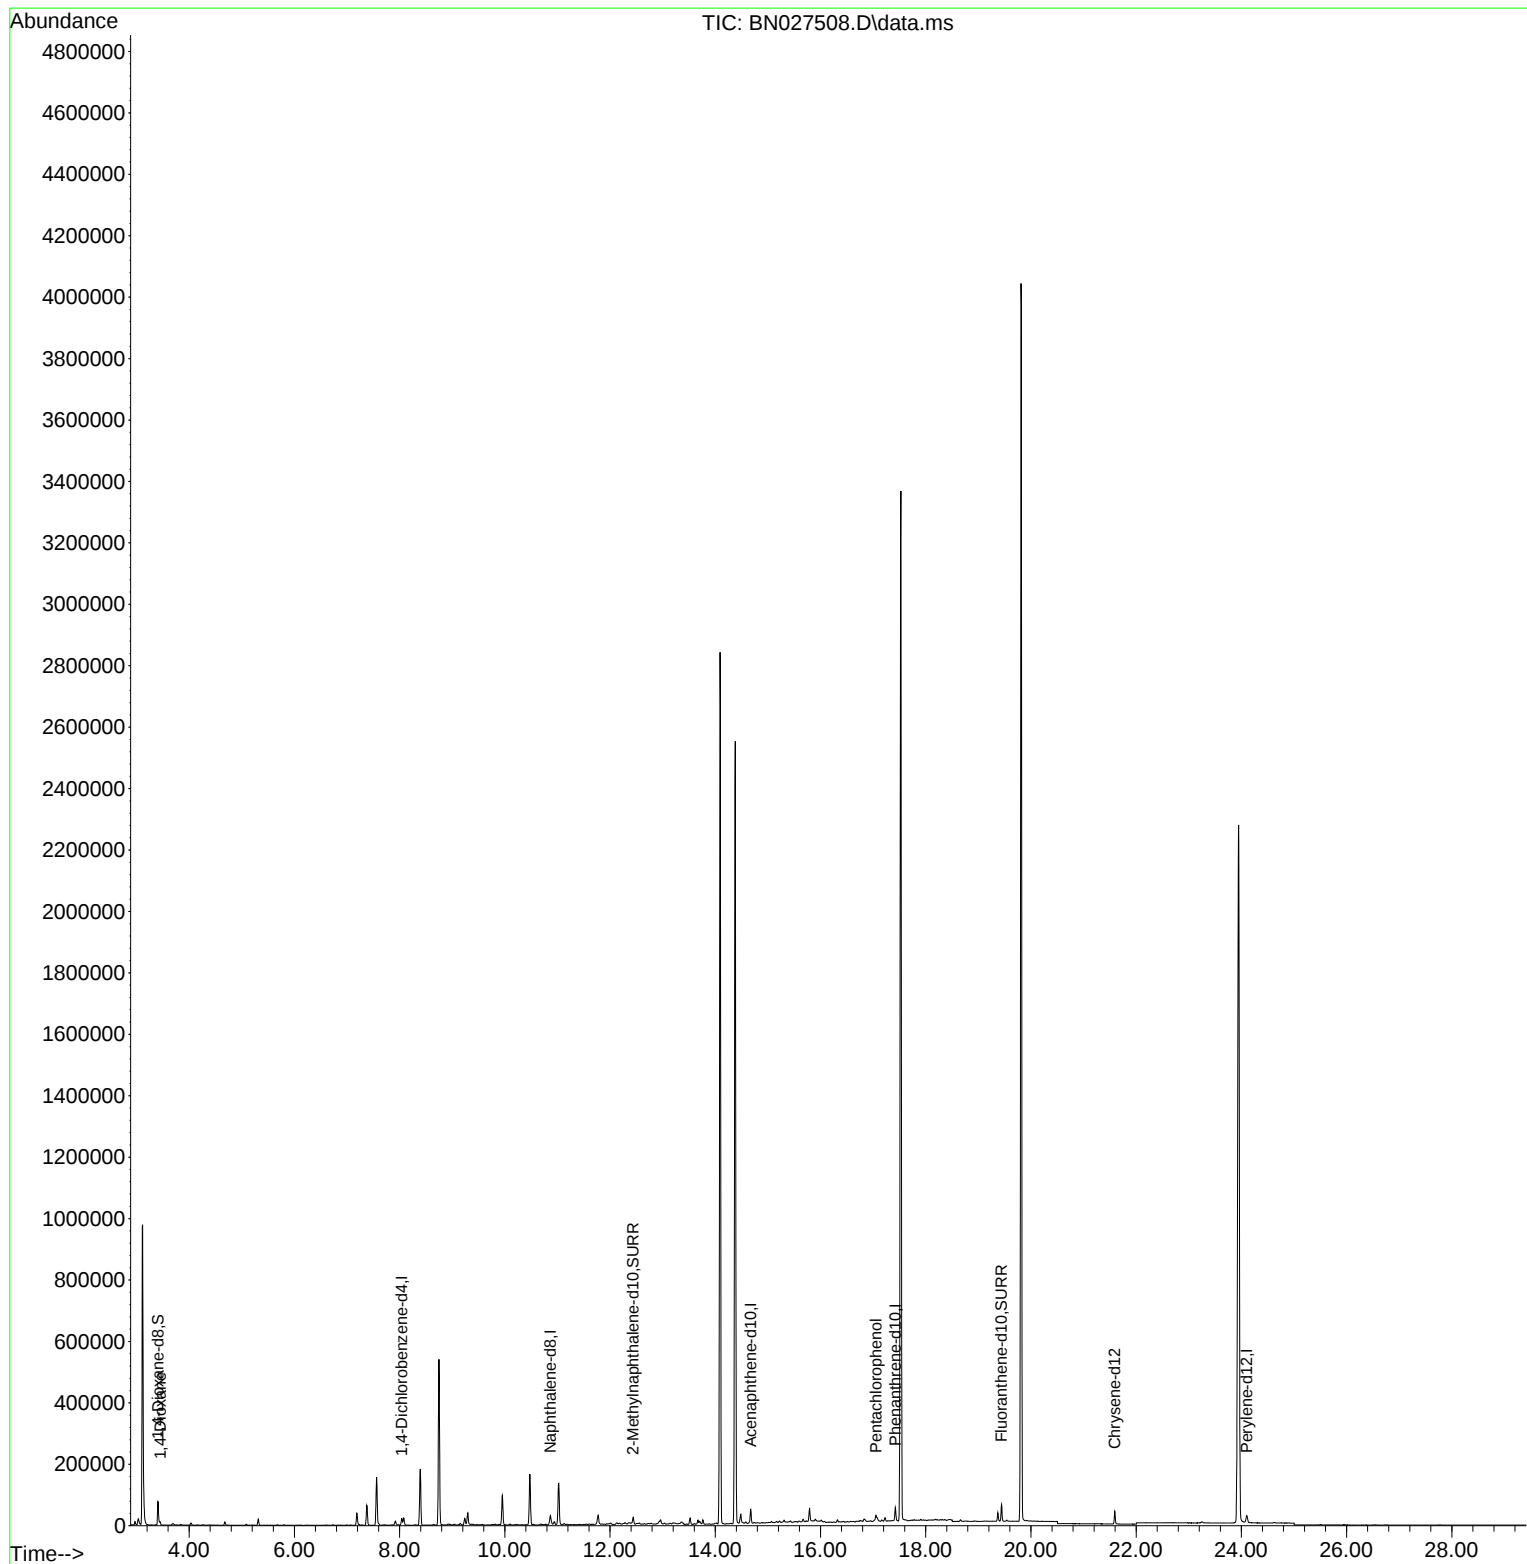


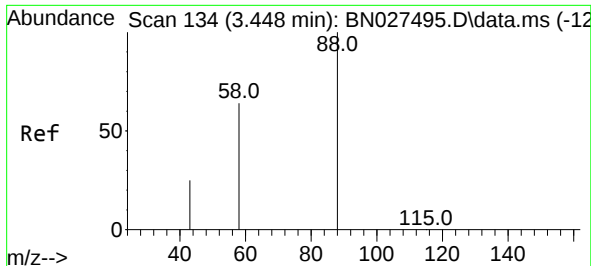

#2
1,4-Dioxane
Concen: 0.491 ng/ul
RT: 3.448 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN027508.D
Acq: 09 Sep 2023 19:04

Instrument :
BNA_N
ClientSampleId :
BBJW6

Tgt Ion: 88 Resp: 7056
Ion Ratio Lower Upper
88 100
43 35.6 26.8 40.2
58 61.7 39.9 59.9#

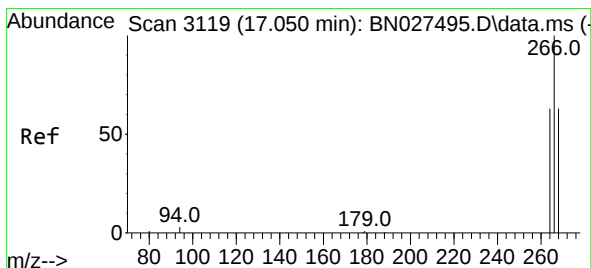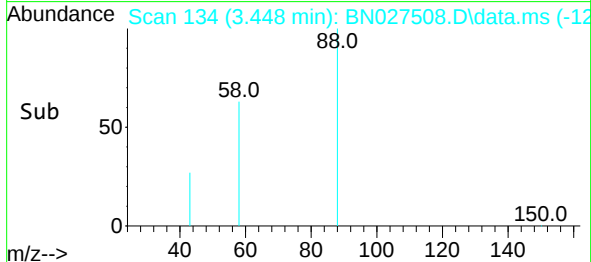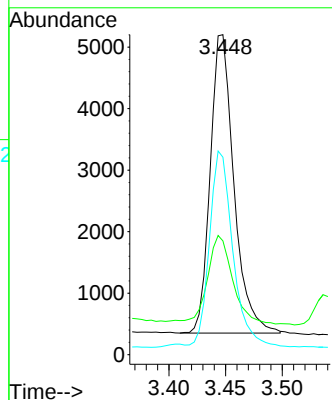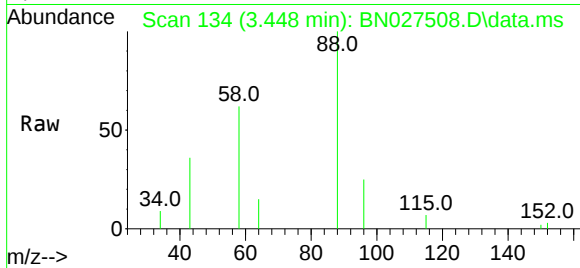

#14
Pentachlorophenol
Concen: 1.238 ng/ul
RT: 17.054 min Scan# 3120
Delta R.T. -0.004 min
Lab File: BN027508.D
Acq: 09 Sep 2023 19:04

Tgt Ion: 266 Resp: 12410
Ion Ratio Lower Upper
266 100
264 62.6 50.4 75.6
268 63.7 51.9 77.9

