

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027514.D
 Acq On : 09 Sep 2023 22:47
 Operator : MA/JU
 Sample : 04227-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH9X8

Quant Time: Sep 10 04:58:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	9216	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	31738	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.675	164	19680	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.421	188	43941	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	32514	0.400	ng/ul	0.00
23) Perylene-d12	24.102	264	30338	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.409	96	42311	3.451	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.439	152	17274	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	48549	0.436	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.447	88	11964	0.964	ng/ul#	87
15) Phenanthrene	17.464	178	8732	0.061	ng/ul	96
20) Pyrene	19.840	202	4098	0.027	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027514.D
Acq On : 09 Sep 2023 22:47
Operator : MA/JU
Sample : 04227-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH9X8

Quant Time: Sep 10 04:58:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




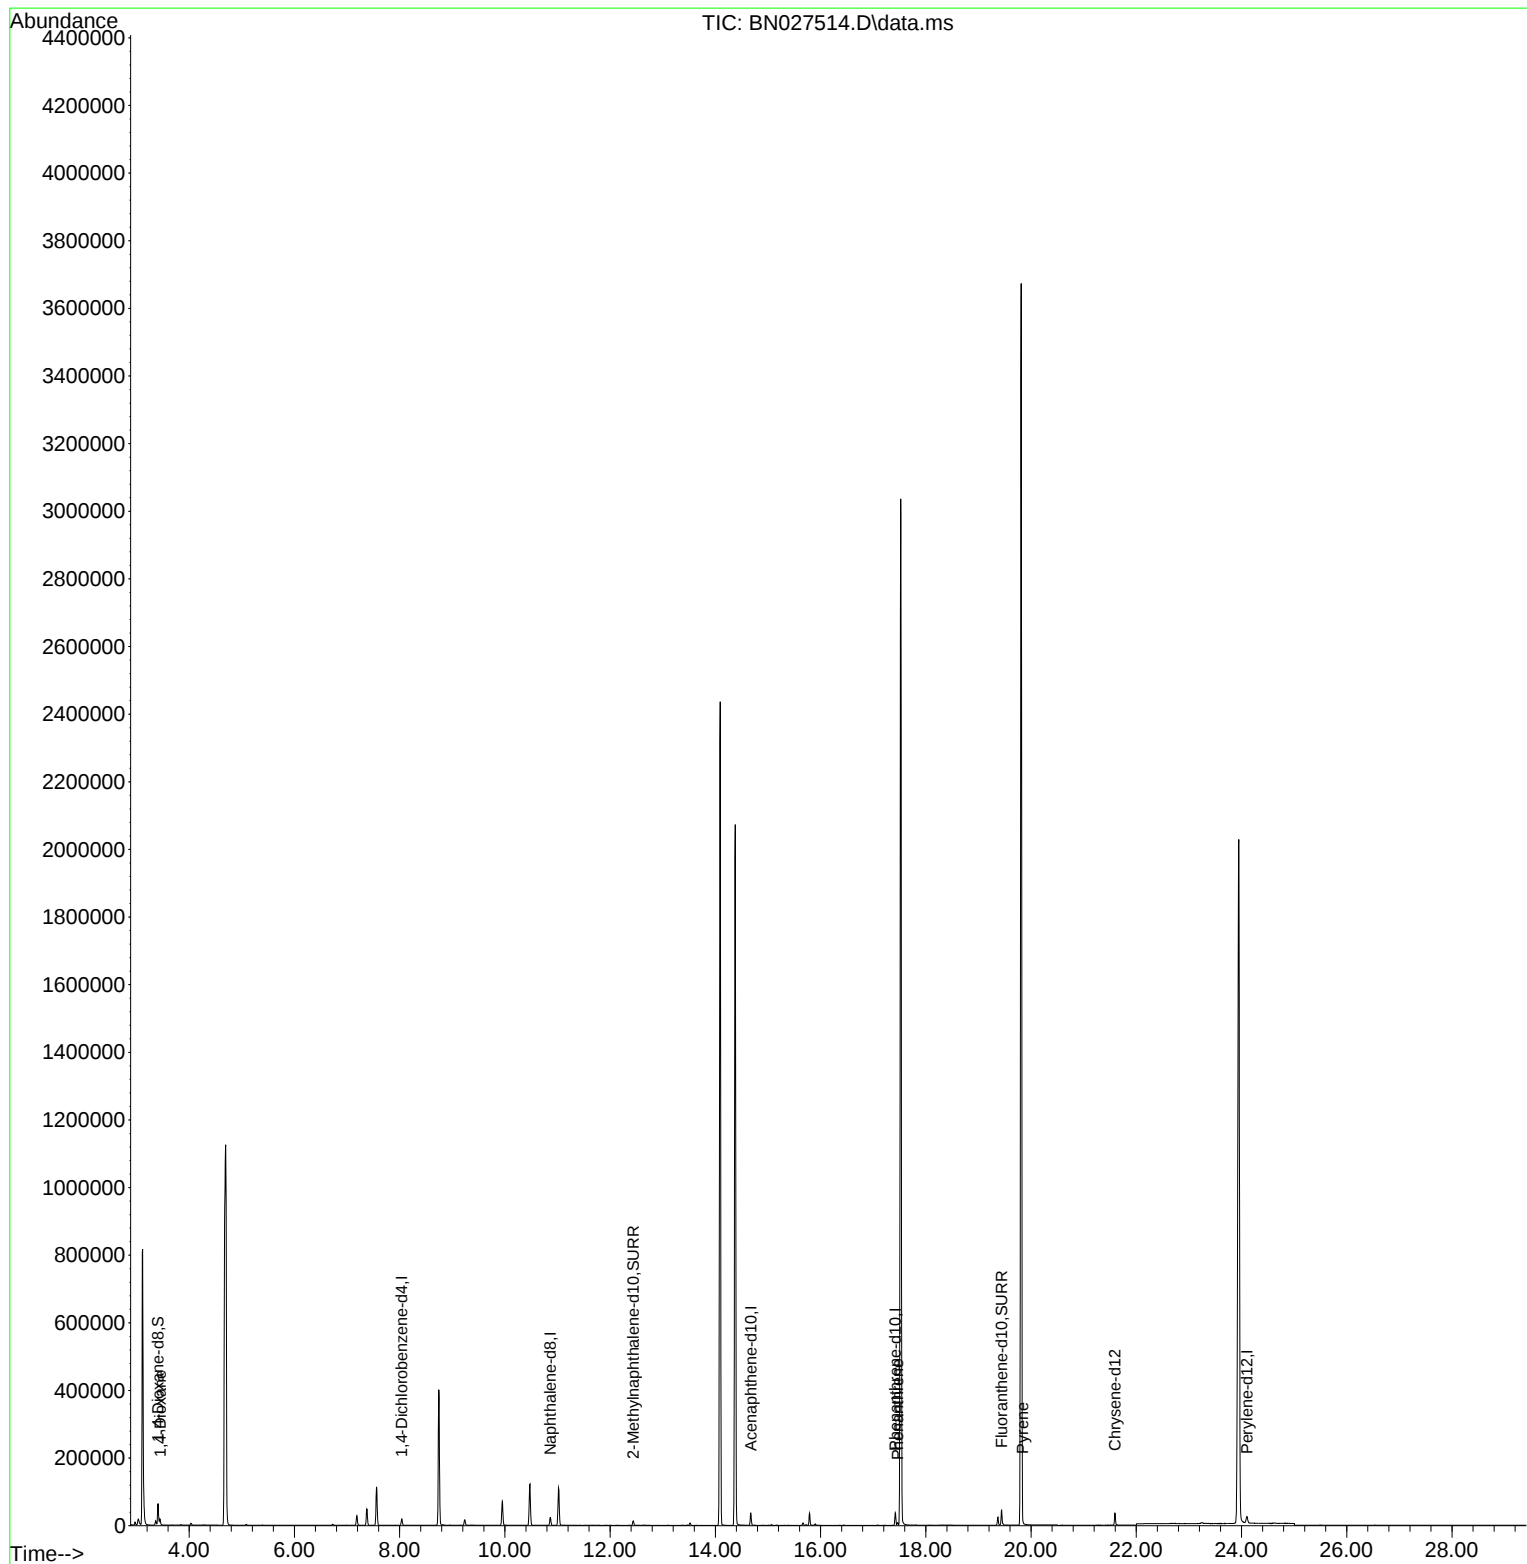


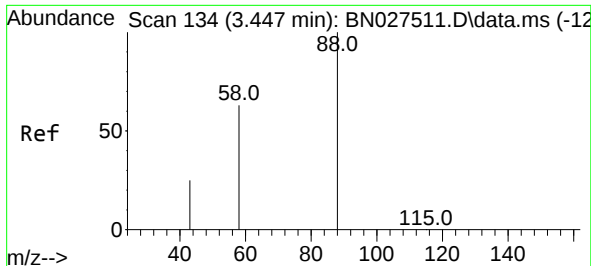

#2
1,4-Dioxane
Concen: 0.964 ng/ul
RT: 3.447 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN027514.D
Acq: 09 Sep 2023 22:47




Instrument :
BNA_N
ClientSampleId :
BH9X8


Tgt Ion: 88 Resp: 11964
Ion Ratio Lower Upper
88 100
43 29.5 26.8 40.2
58 61.8 39.9 59.9#

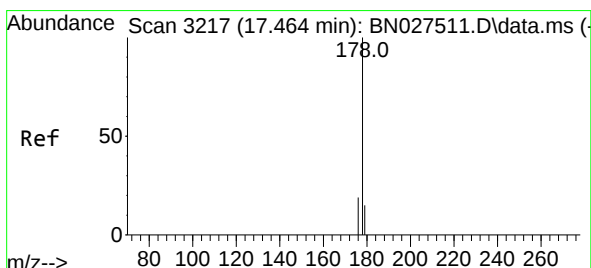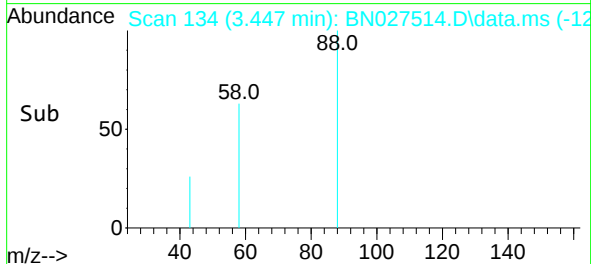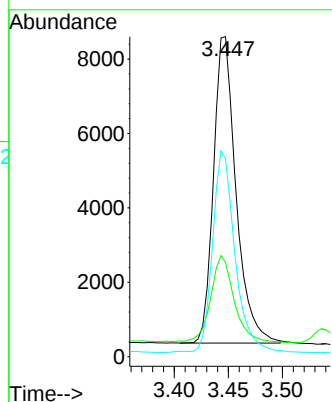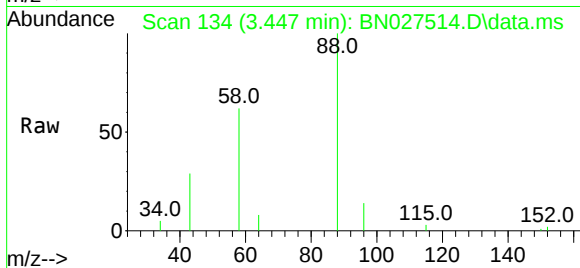

#15
Phenanthrene
Concen: 0.061 ng/ul
RT: 17.464 min Scan# 3217
Delta R.T. -0.005 min
Lab File: BN027514.D
Acq: 09 Sep 2023 22:47

Tgt Ion: 178 Resp: 8732
Ion Ratio Lower Upper
178 100
179 18.2 12.6 19.0
176 21.3 15.8 23.8

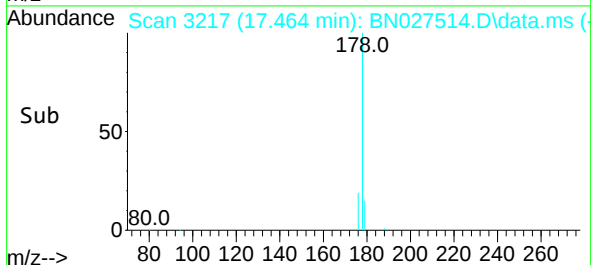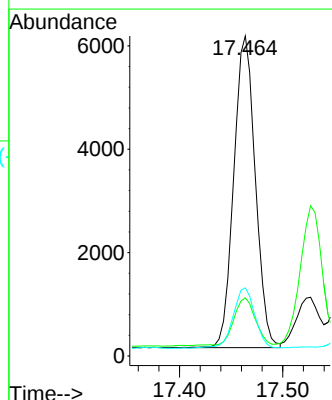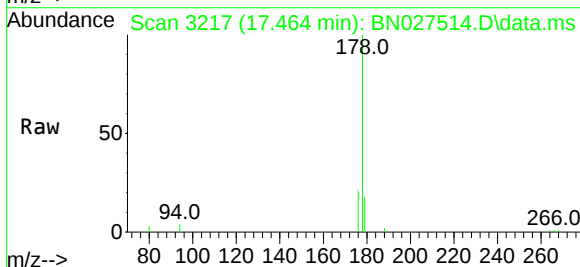

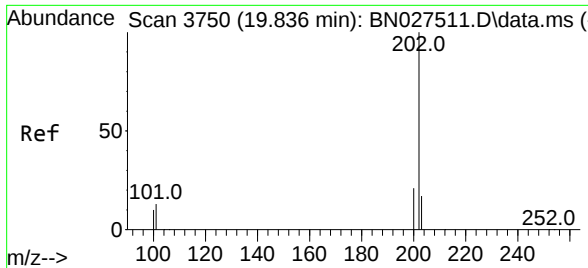

#20
 Pyrene
 Concen: 0.027 ng/ul
 RT: 19.840 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN027514.D
 Acq: 09 Sep 2023 22:47

Instrument :
 BNA_N
 ClientSampleId :
 BH9X8

Tgt Ion:202 Resp: 4098
 Ion Ratio Lower Upper
 202 100
 101 16.9 11.4 17.2
 100 17.2 9.4 14.2#

