

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027517.D
 Acq On : 10 Sep 2023 00:40
 Operator : MA/JU
 Sample : 04227-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKJ7

Quant Time: Sep 10 05:01:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	7489	0.400	ng/ul	0.00
4) Naphthalene-d8	10.867	136	26023	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.675	164	19723	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	35306	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.595	240	23353	0.400	ng/ul	0.00
23) Perylene-d12	24.103	264	20809	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	42588	4.275	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	19566	0.495	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	45241	0.565	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.443	88	36110	3.582	ng/ul#	85
14) Pentachlorophenol	17.050	266	11945	1.735	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027517.D
Acq On : 10 Sep 2023 00:40
Operator : MA/JU
Sample : 04227-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKJ7

Quant Time: Sep 10 05:01:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration




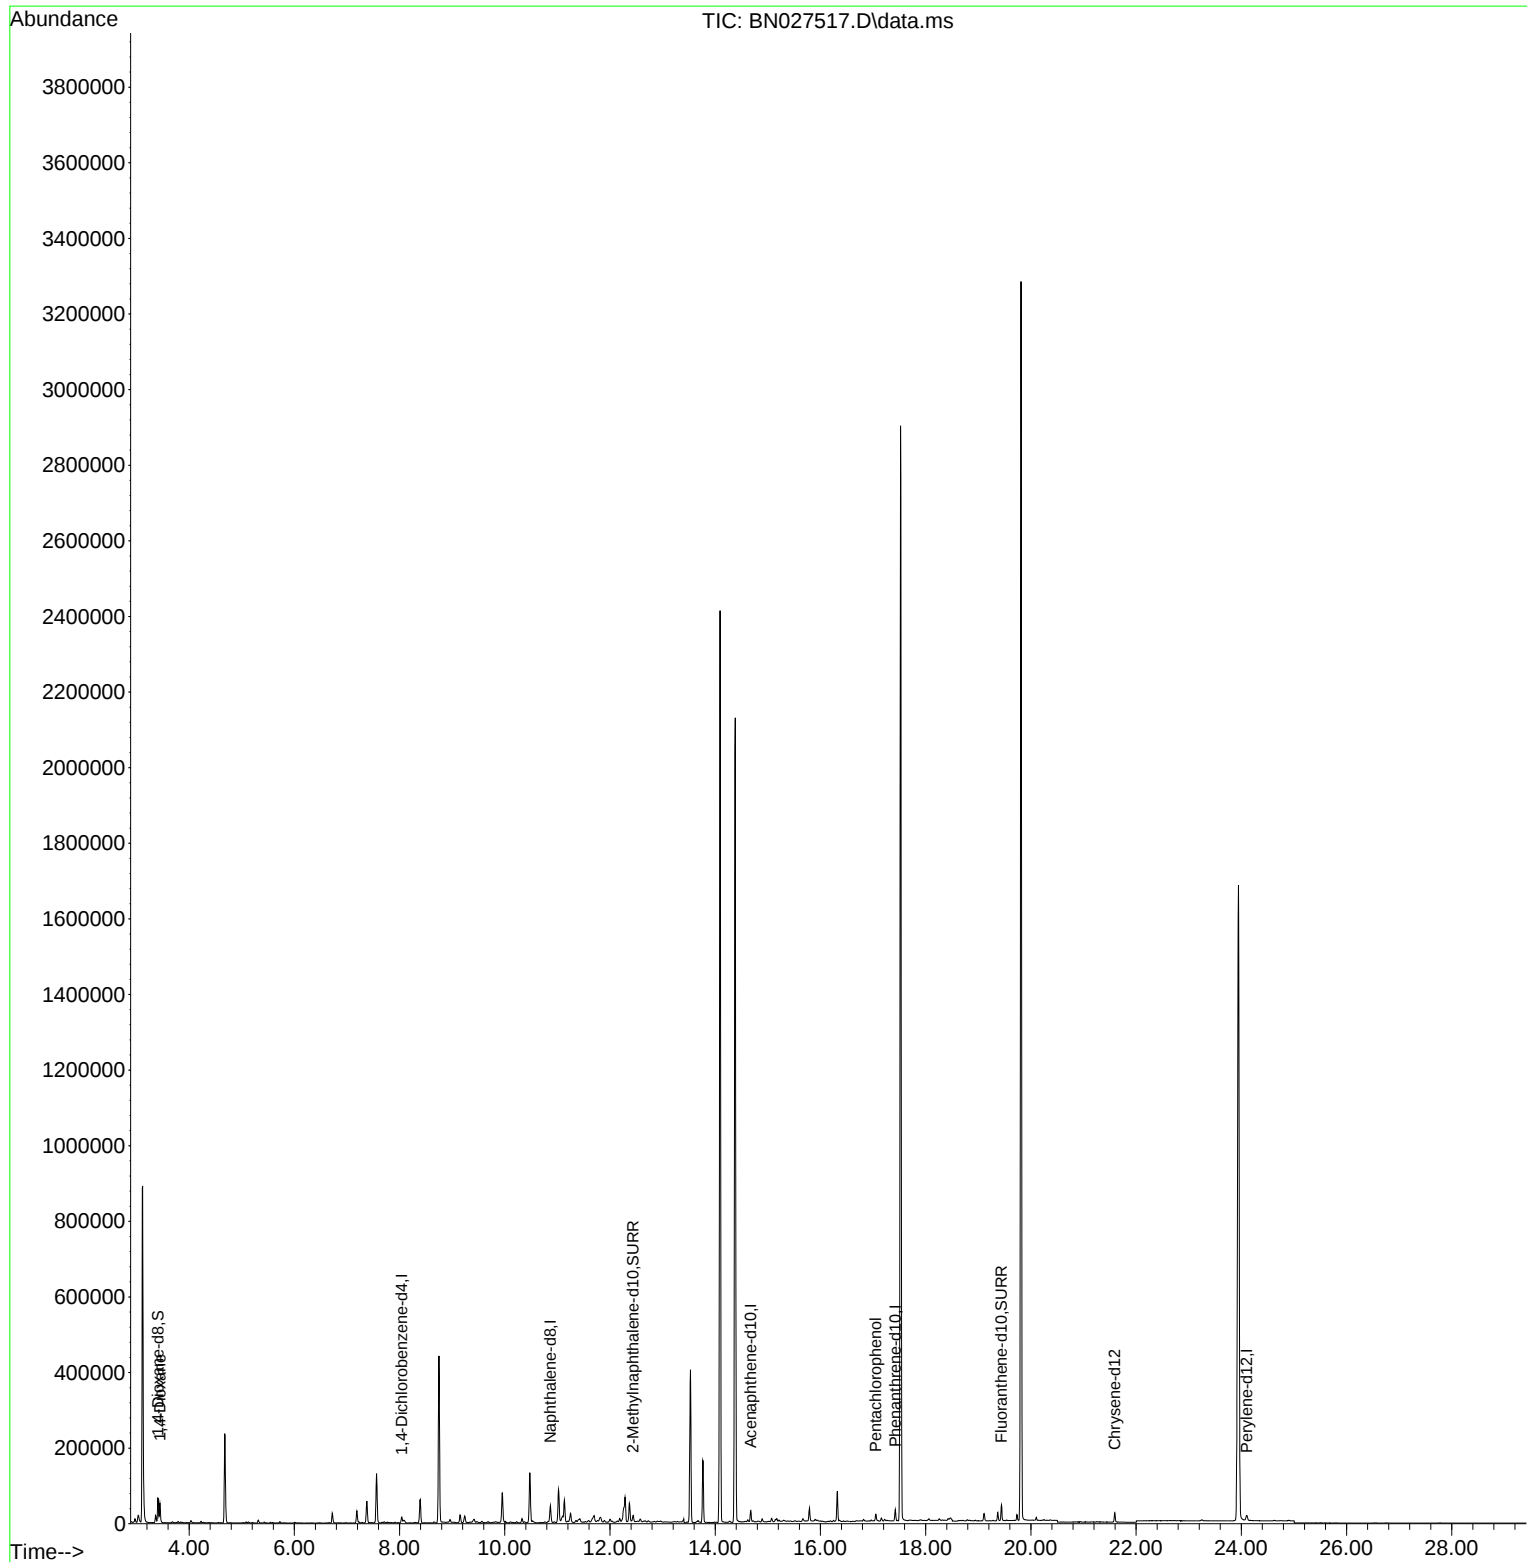


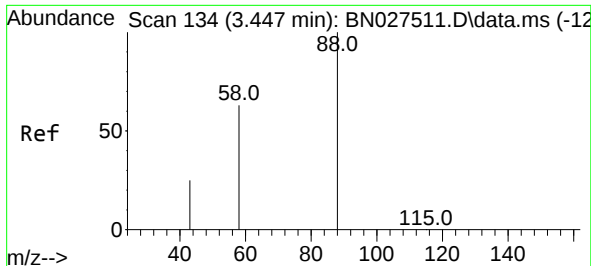

#2
1,4-Dioxane
Concen: 3.582 ng/ul
RT: 3.443 min Scan# 111
Delta R.T. -0.004 min
Lab File: BN027517.D
Acq: 10 Sep 2023 00:40

Instrument :
BNA_N
ClientSampleId :
BBKJ7

Tgt Ion: 88 Resp: 36110
Ion Ratio Lower Upper
88 100
43 30.8 26.8 40.2
58 65.5 39.9 59.9#

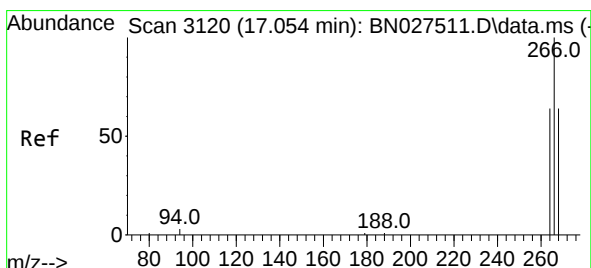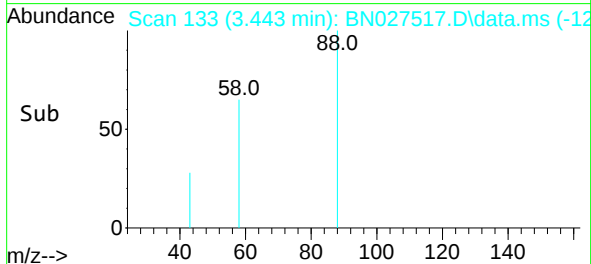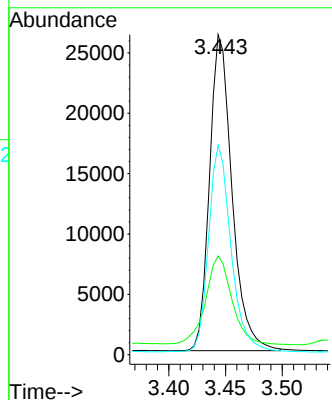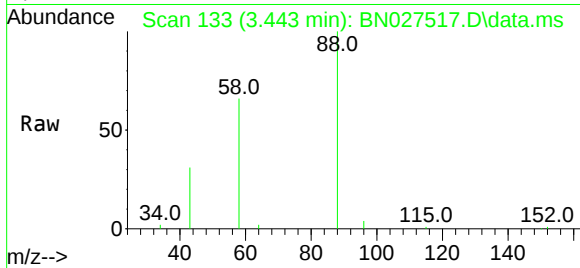

#14
Pentachlorophenol
Concen: 1.735 ng/ul
RT: 17.050 min Scan# 3119
Delta R.T. -0.009 min
Lab File: BN027517.D
Acq: 10 Sep 2023 00:40

Tgt Ion: 266 Resp: 11945
Ion Ratio Lower Upper
266 100
264 63.0 50.4 75.6
268 63.8 51.9 77.9

