

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027518.D
 Acq On : 10 Sep 2023 01:18
 Operator : MA/JU
 Sample : 04227-17
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKF2

Quant Time: Sep 10 05:02:01 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.042	152	7849	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	27090	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164	17000	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	37679	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	28153	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	27026	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.410	96	38110	3.650	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	16081	0.391	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	43473	0.451	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	1581	0.150	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027518.D
Acq On : 10 Sep 2023 01:18
Operator : MA/JU
Sample : 04227-17
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKF2

Quant Time: Sep 10 05:02:01 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

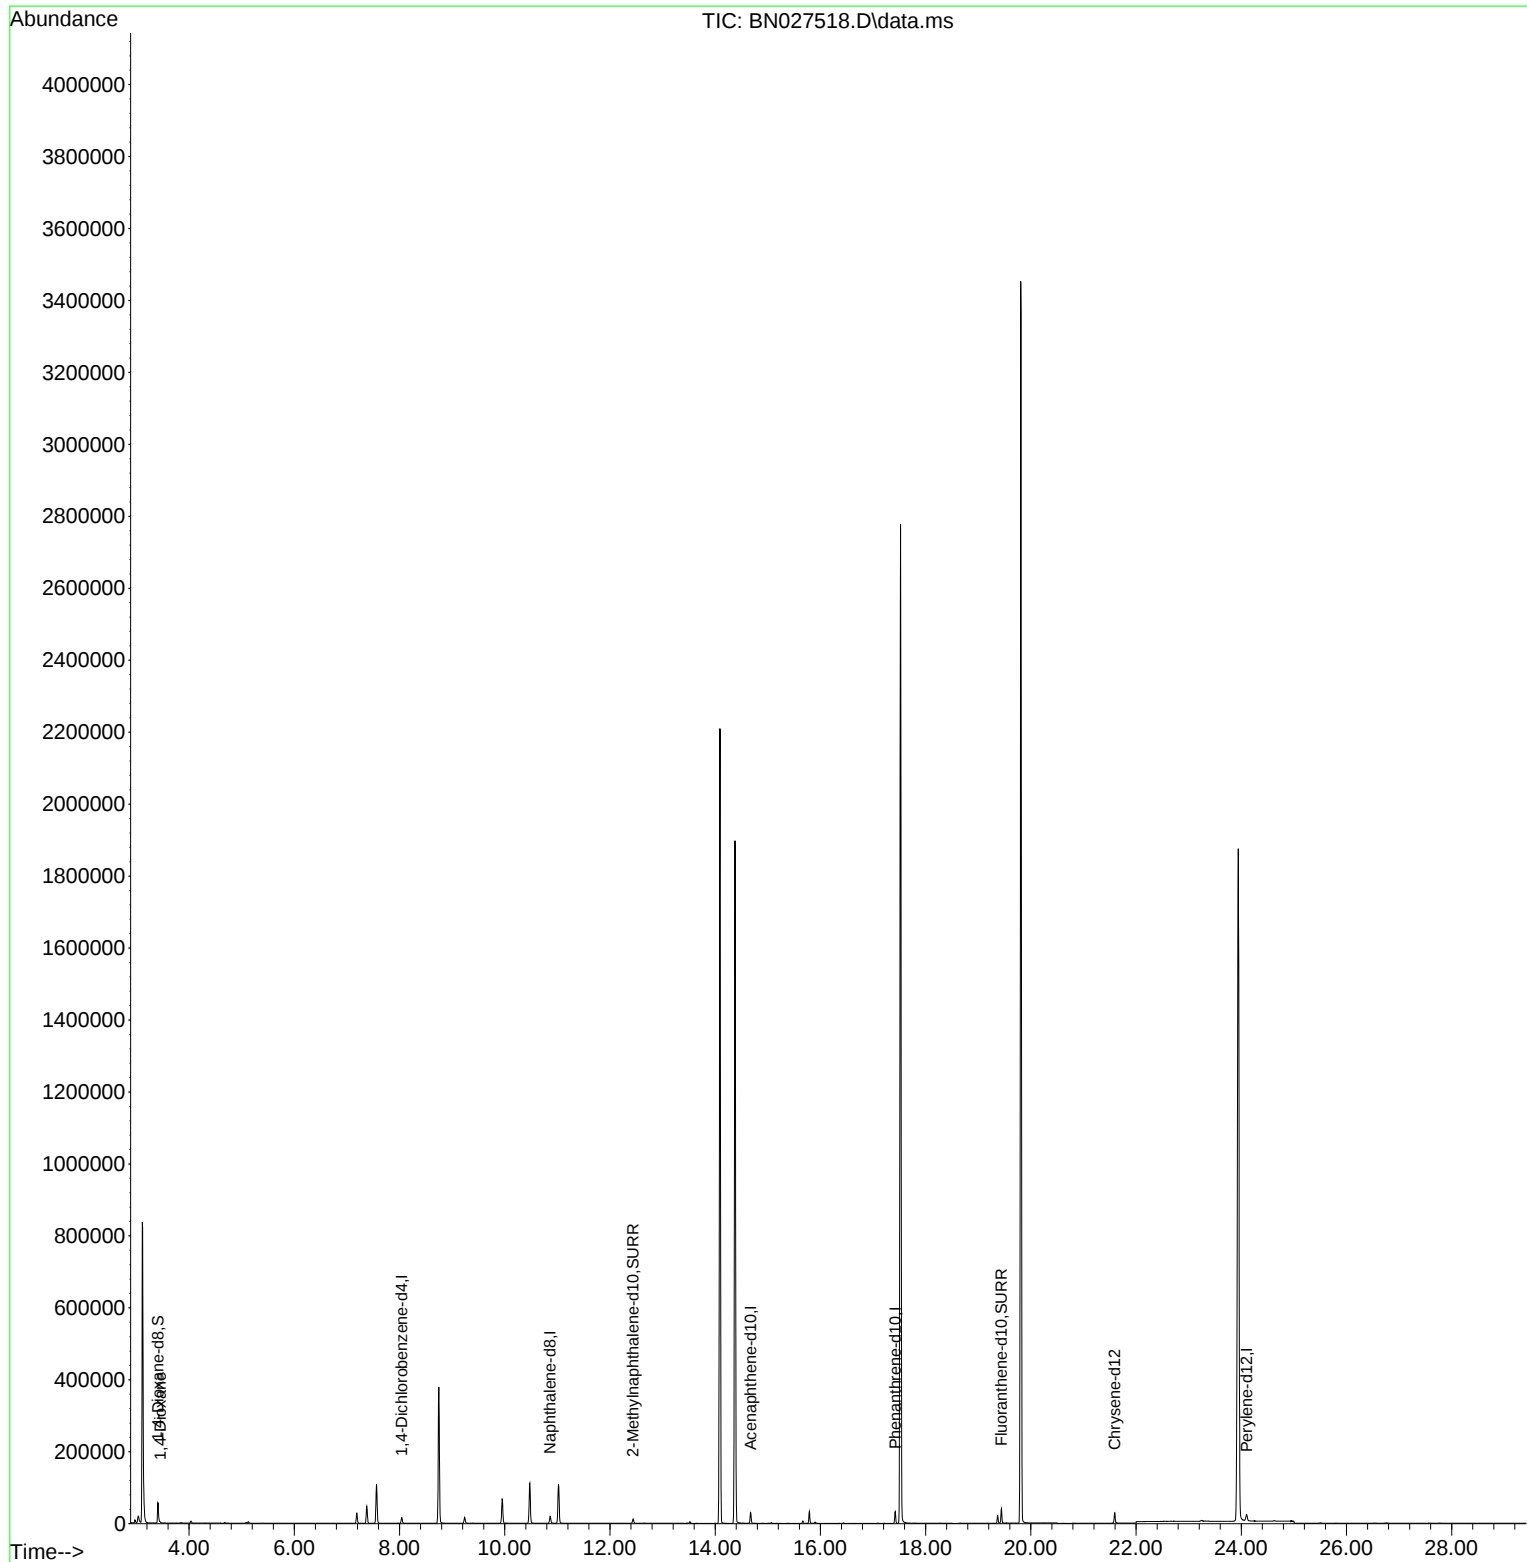

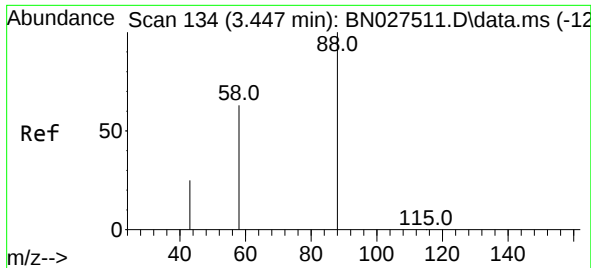

1,4-Dioxane

Concen: 0.150 ng/ul

RT: 3.448 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN027518.D

Acq: 10 Sep 2023 01:18

Instrument :

BNA_N

ClientSampleId :

BBKF2

Tgt Ion: 88 Resp: 1581

Ion Ratio Lower Upper

88 100

43 51.2 26.8 40.2#

58 56.8 39.9 59.9

