

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027520.D
 Acq On : 10 Sep 2023 02:32
 Operator : MA/JU
 Sample : 04227-19
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ99

Quant Time: Sep 10 05:04:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	9672	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	33744	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.670	164	21209	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	46502	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	33760	0.400	ng/ul	0.00
23) Perylene-d12	24.100	264	32201	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	52726	4.098	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	20851	0.407	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	51936	0.449	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.443	88	2468	0.190	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027520.D
Acq On : 10 Sep 2023 02:32
Operator : MA/JU
Sample : 04227-19
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ99

Quant Time: Sep 10 05:04:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

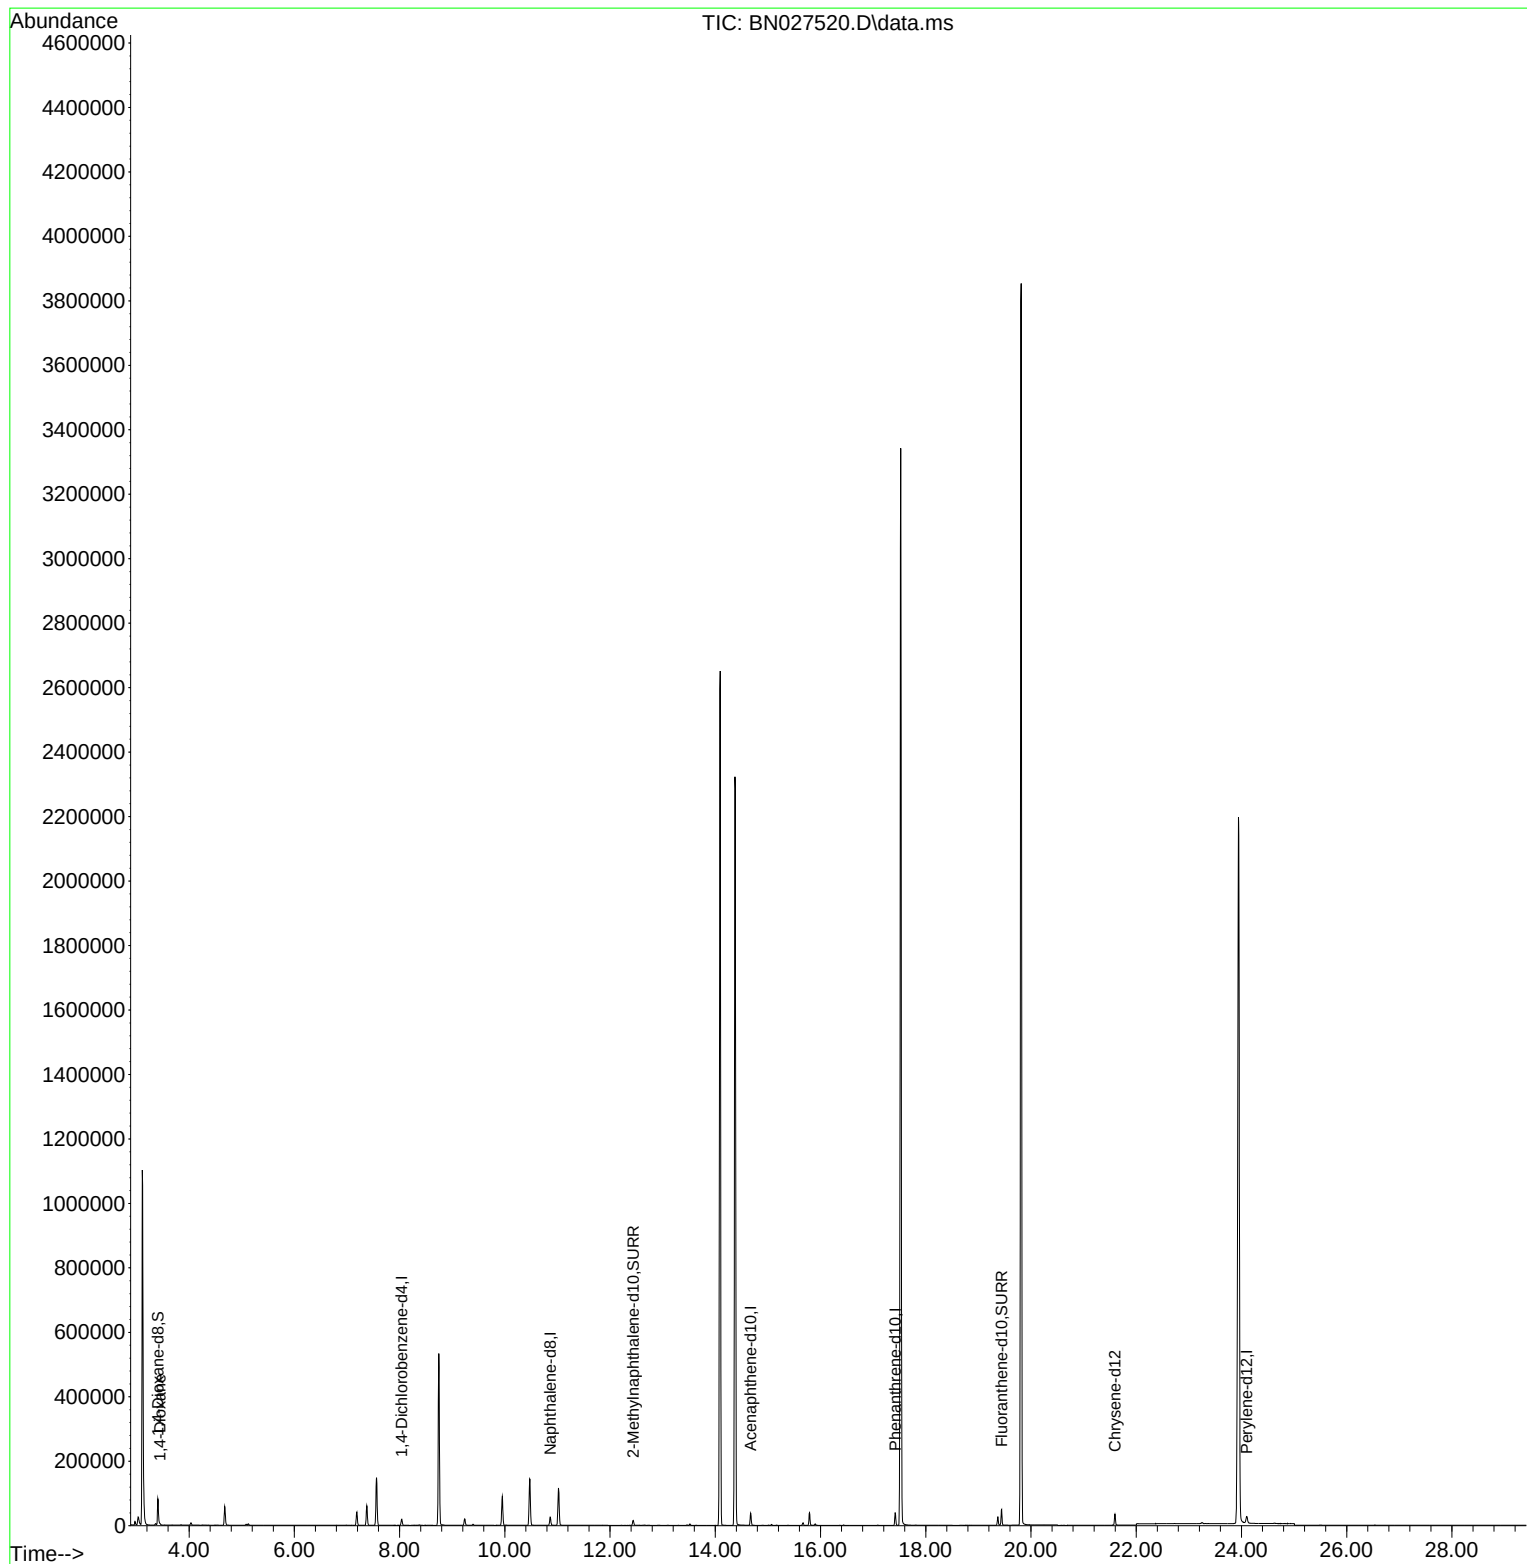

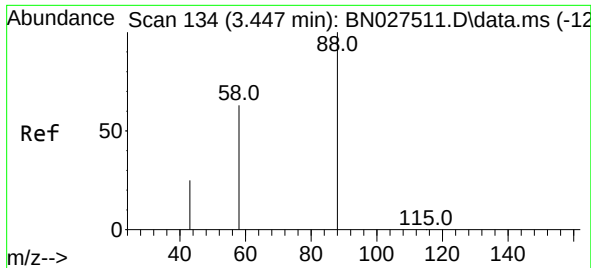

#2
 1,4-Dioxane
 Concen: 0.190 ng/ul
 RT: 3.443 min Scan# 11
 Delta R.T. -0.004 min
 Lab File: BN027520.D
 Acq: 10 Sep 2023 02:32

Instrument :
 BNA_N
 ClientSampleId :
 BBJ99

Tgt Ion: 88 Resp: 2468
 Ion Ratio Lower Upper
 88 100
 43 43.3 26.8 40.2#
 58 60.7 39.9 59.9#

