

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027521.D
 Acq On : 10 Sep 2023 03:09
 Operator : MA/JU
 Sample : 04227-20
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ92

Quant Time: Sep 10 05:05:29 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	8622	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	30034	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164	18342	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.422	188	39949	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	28709	0.400	ng/ul	0.00
23) Perylene-d12	24.099	264	26942	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	42419	3.699	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.440	152	16805	0.369	ng/ul	0.00
18) Fluoranthene-d10	19.441	212	42978	0.437	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.448	88	2026	0.175	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027521.D
Acq On : 10 Sep 2023 03:09
Operator : MA/JU
Sample : 04227-20
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ92

Quant Time: Sep 10 05:05:29 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

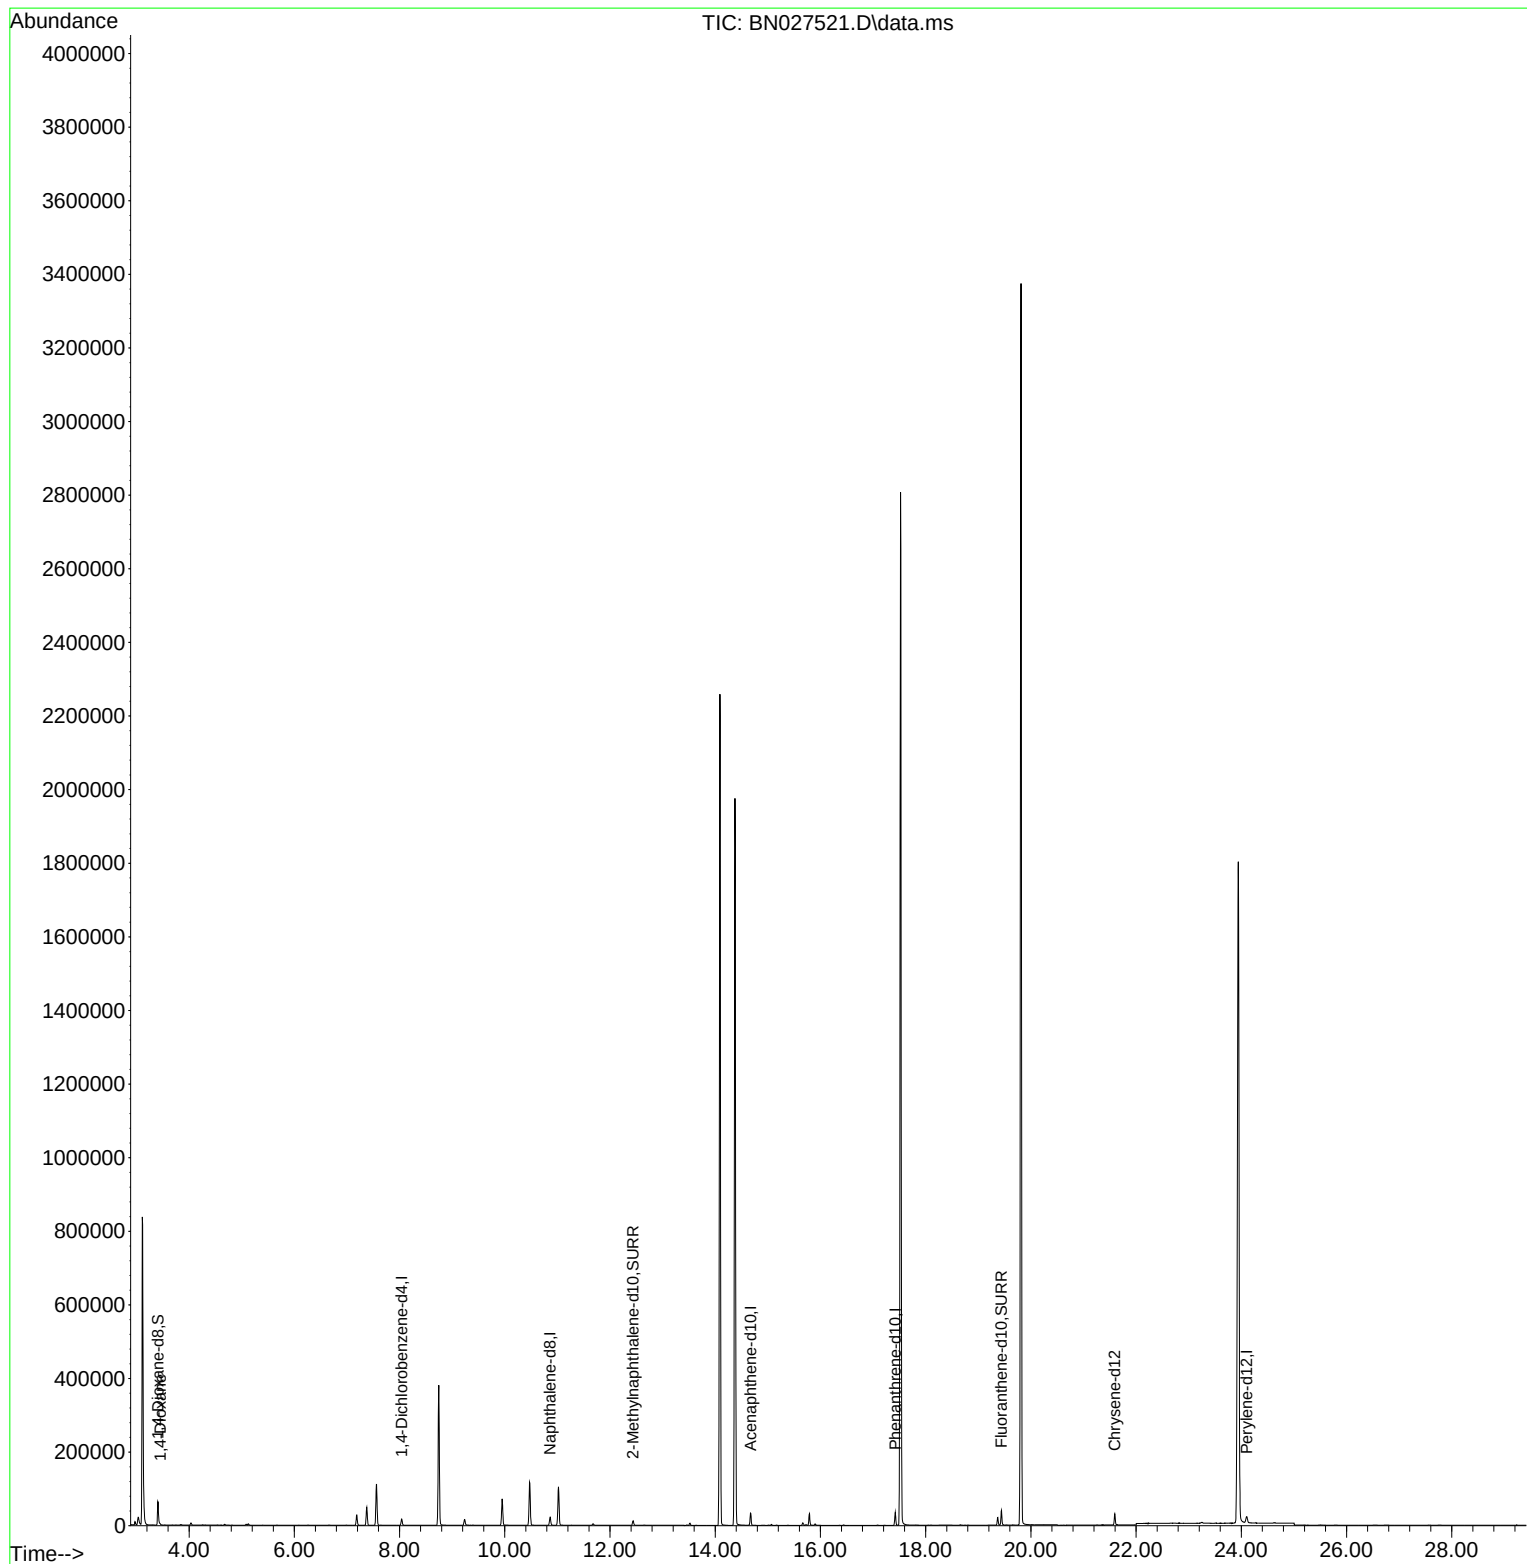

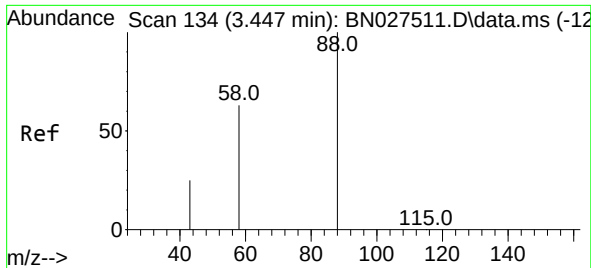

#2
 1,4-Dioxane
 Concen: 0.175 ng/ul
 RT: 3.448 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BN027521.D
 Acq: 10 Sep 2023 03:09

Instrument :
 BNA_N
 ClientSampleId :
 BBJ92

Tgt Ion: 88 Resp: 2026

Ion	Ratio	Lower	Upper
88	100		
43	43.9	26.8	40.2#
58	56.8	39.9	59.9

