

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027533.D
 Acq On : 10 Sep 2023 10:31
 Operator : MA/JU
 Sample : 04250-02
 Misc :
 ALS Vial : 41 Sample Multiplier: 1


Instrument :
 BNA_N
 ClientSampleId :
 BH4A1

Quant Time: Sep 11 01:18:33 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	7430	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	24832	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164	15643	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.418	188	32301	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.595	240	22184	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	20078	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	37361	3.780	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	11599	0.308	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	26858	0.353	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	893	0.089	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

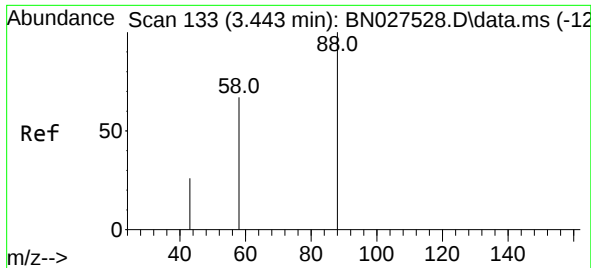

1,4-Dioxane

Concen: 0.089 ng/ul

RT: 3.444 min Scan# 11

Delta R.T. -0.004 min

Lab File: BN027533.D


Acq: 10 Sep 2023 10:31

Instrument :

BNA_N

ClientSampleId :

BH4A1



Tgt Ion: 88 Resp: 893

Ion Ratio Lower Upper

88 100

43 308.6 26.8 40.2#

58 124.3 39.9 59.9#

