

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027534.D
 Acq On : 10 Sep 2023 11:08
 Operator : MA/JU
 Sample : 04250-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH4A3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2023
 Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 11 01:18:39 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.038	152	6508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.861	136	22539	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.671	164	14158	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.418	188	31274	0.400	ng/ul	0.00
17) Chrysene-d12	21.595	240	21467	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	20130	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	46168m	5.333	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	12488	0.365	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	30488	0.415	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	1376	0.157	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027534.D
Acq On : 10 Sep 2023 11:08
Operator : MA/JU
Sample : 04250-04
Misc :
ALS Vial : 42 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BH4A3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2023
Supervised By :mohammad ahmed 09/11/2023

Quant Time: Sep 11 01:18:39 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

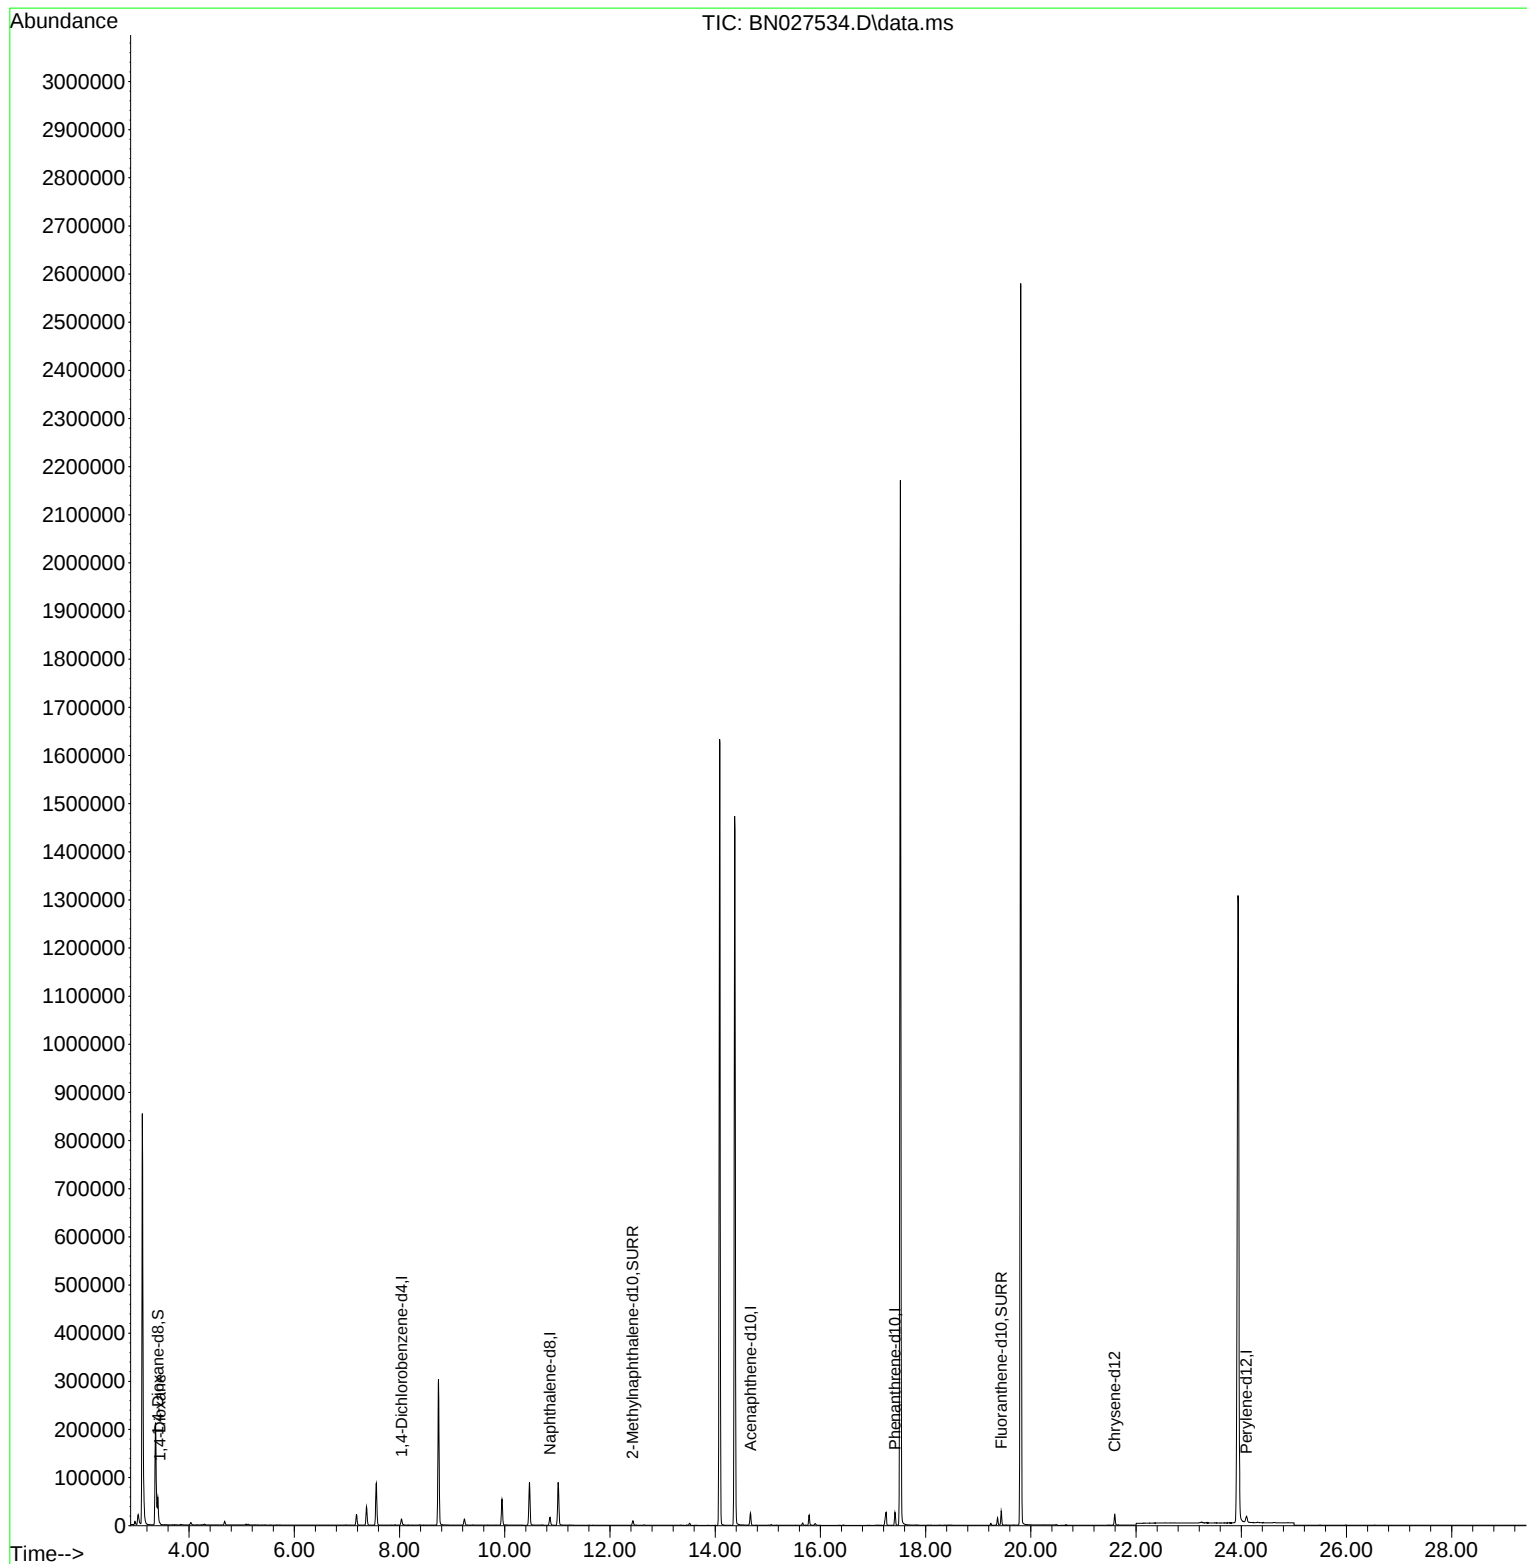

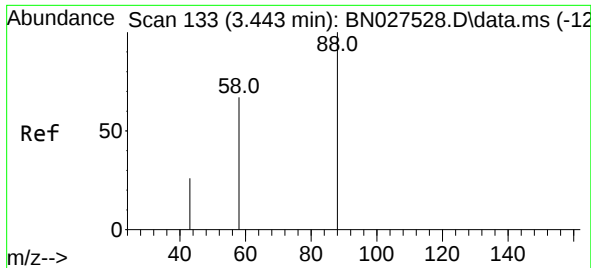

1,4-Dioxane

Concen: 0.157 ng/ul

RT: 3.444 min Scan# 11

Delta R.T. -0.004 min

Lab File: BN027534.D

Acq: 10 Sep 2023 11:08

Instrument :

BNA_N

ClientSampleId :

BH4A3

Tgt Ion: 88 Resp: 1370

Ion Ratio Lower Upper

88 100

43 54.6 26.8 40.2

58 57.1 39.9 59.9

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 09/11/2023

Supervised By :mohammad ahmed 09/11/2023

