

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027547.D
 Acq On : 10 Sep 2023 19:06
 Operator : MA/JU
 Sample : 04262-01
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBJ75

Quant Time: Sep 11 01:20:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	6436	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136	22137	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	13489	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.417	188	28781	0.400	ng/ul	0.00
17) Chrysene-d12	21.594	240	19662	0.400	ng/ul	0.00
23) Perylene-d12	24.097	264	17467	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	39384	4.600	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	10350	0.308	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	26203	0.389	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.444	88	27299	3.151	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027547.D
Acq On : 10 Sep 2023 19:06
Operator : MA/JU
Sample : 04262-01
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBJ75


Quant Time: Sep 11 01:20:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

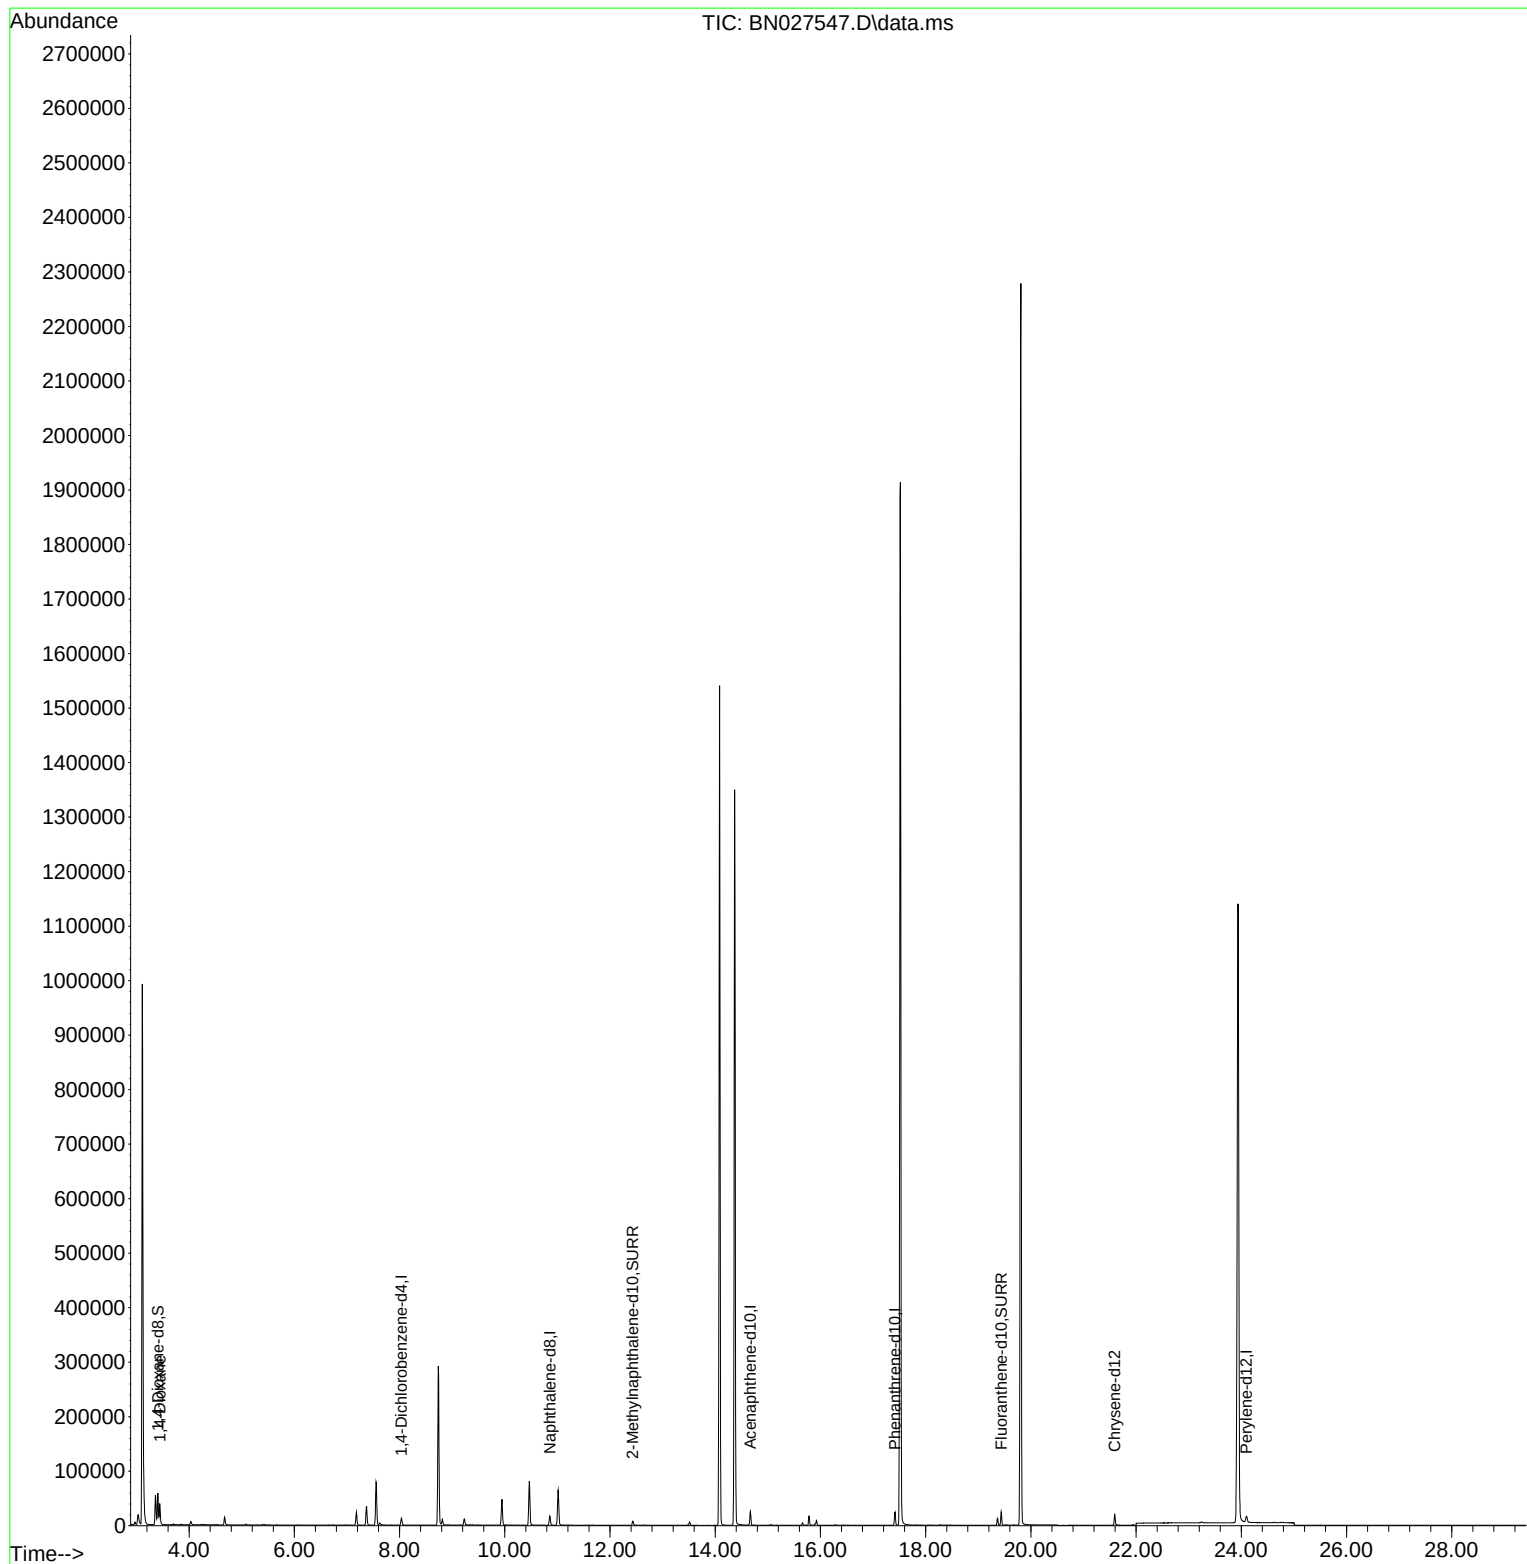

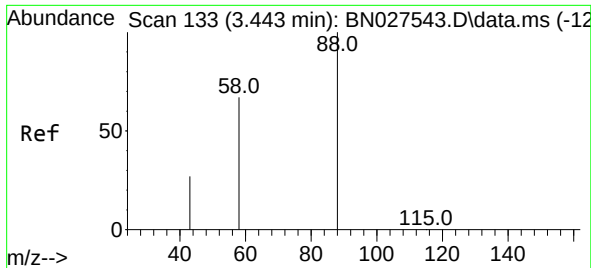

#2
 1,4-Dioxane
 Concen: 3.151 ng/ul
 RT: 3.444 min Scan# 11
 Delta R.T. -0.004 min
 Lab File: BN027547.D
 Acq: 10 Sep 2023 19:06

Instrument :
 BNA_N
 ClientSampleId :
 BBJ75

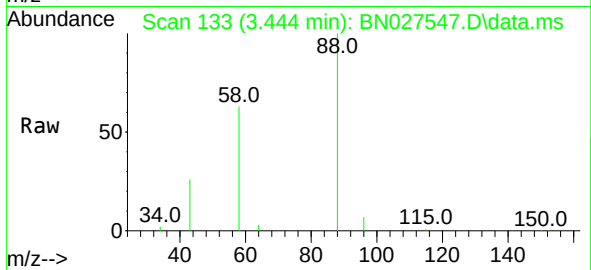

Tgt Ion: 88 Resp: 27299
 Ion Ratio Lower Upper
 88 100
 43 26.3 26.8 40.2#
 58 63.3 39.9 59.9#

