

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
 Data File : BN027548.D
 Acq On : 10 Sep 2023 19:43
 Operator : MA/JU
 Sample : 04262-02
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BBKG1

Quant Time: Sep 11 01:20:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 08 03:55:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	6315	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.856	136	21659	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.666	164	12982	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.418	188	28383	0.400	ng/ul	0.00
17) Chrysene-d12	21.592	240	20413	0.400	ng/ul	0.00
23) Perylene-d12	24.094	264	18861	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.406	96	37744	4.493	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.434	152	11549	0.351	ng/ul	-0.01
18) Fluoranthene-d10	19.436	212	29970	0.429	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.443	88	5528	0.650	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN090923\
Data File : BN027548.D
Acq On : 10 Sep 2023 19:43
Operator : MA/JU
Sample : 04262-02
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BBKG1

Quant Time: Sep 11 01:20:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 08 03:55:54 2023
Response via : Initial Calibration

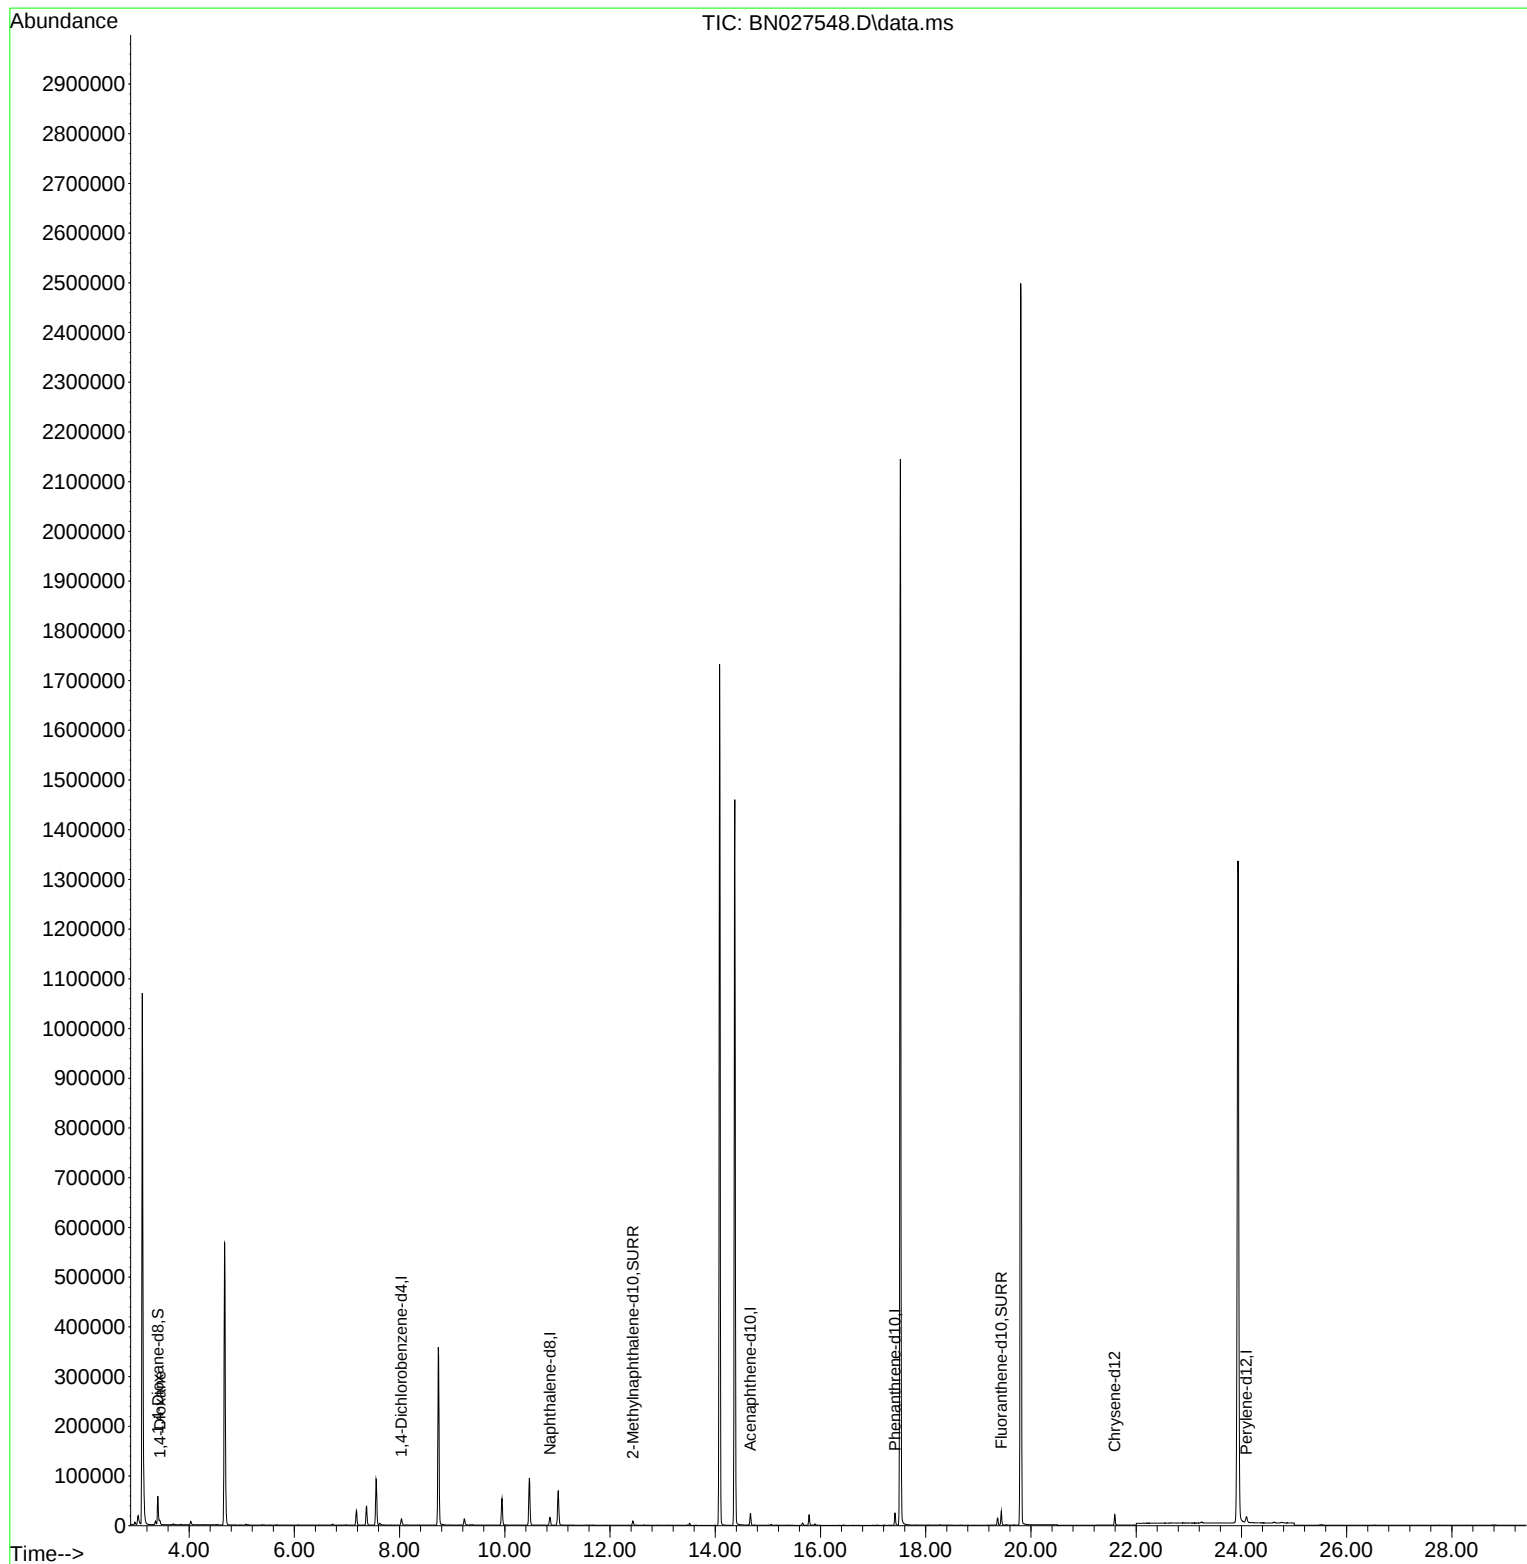

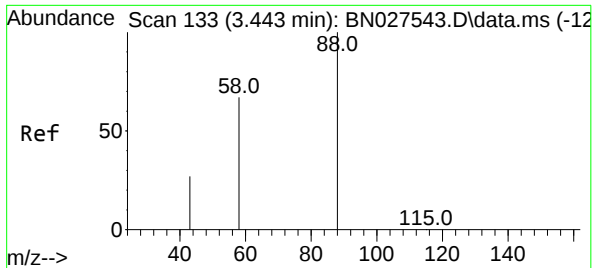

#2
1,4-Dioxane
Concen: 0.650 ng/ul
RT: 3.443 min Scan# 11
Delta R.T. -0.004 min
Lab File: BN027548.D
Acq: 10 Sep 2023 19:43

Instrument :
BNA_N
ClientSampleId :
BBKG1

Tgt Ion: 88 Resp: 5528
Ion Ratio Lower Upper
88 100
43 33.8 26.8 40.2
58 62.1 39.9 59.9#

